




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jan 2020

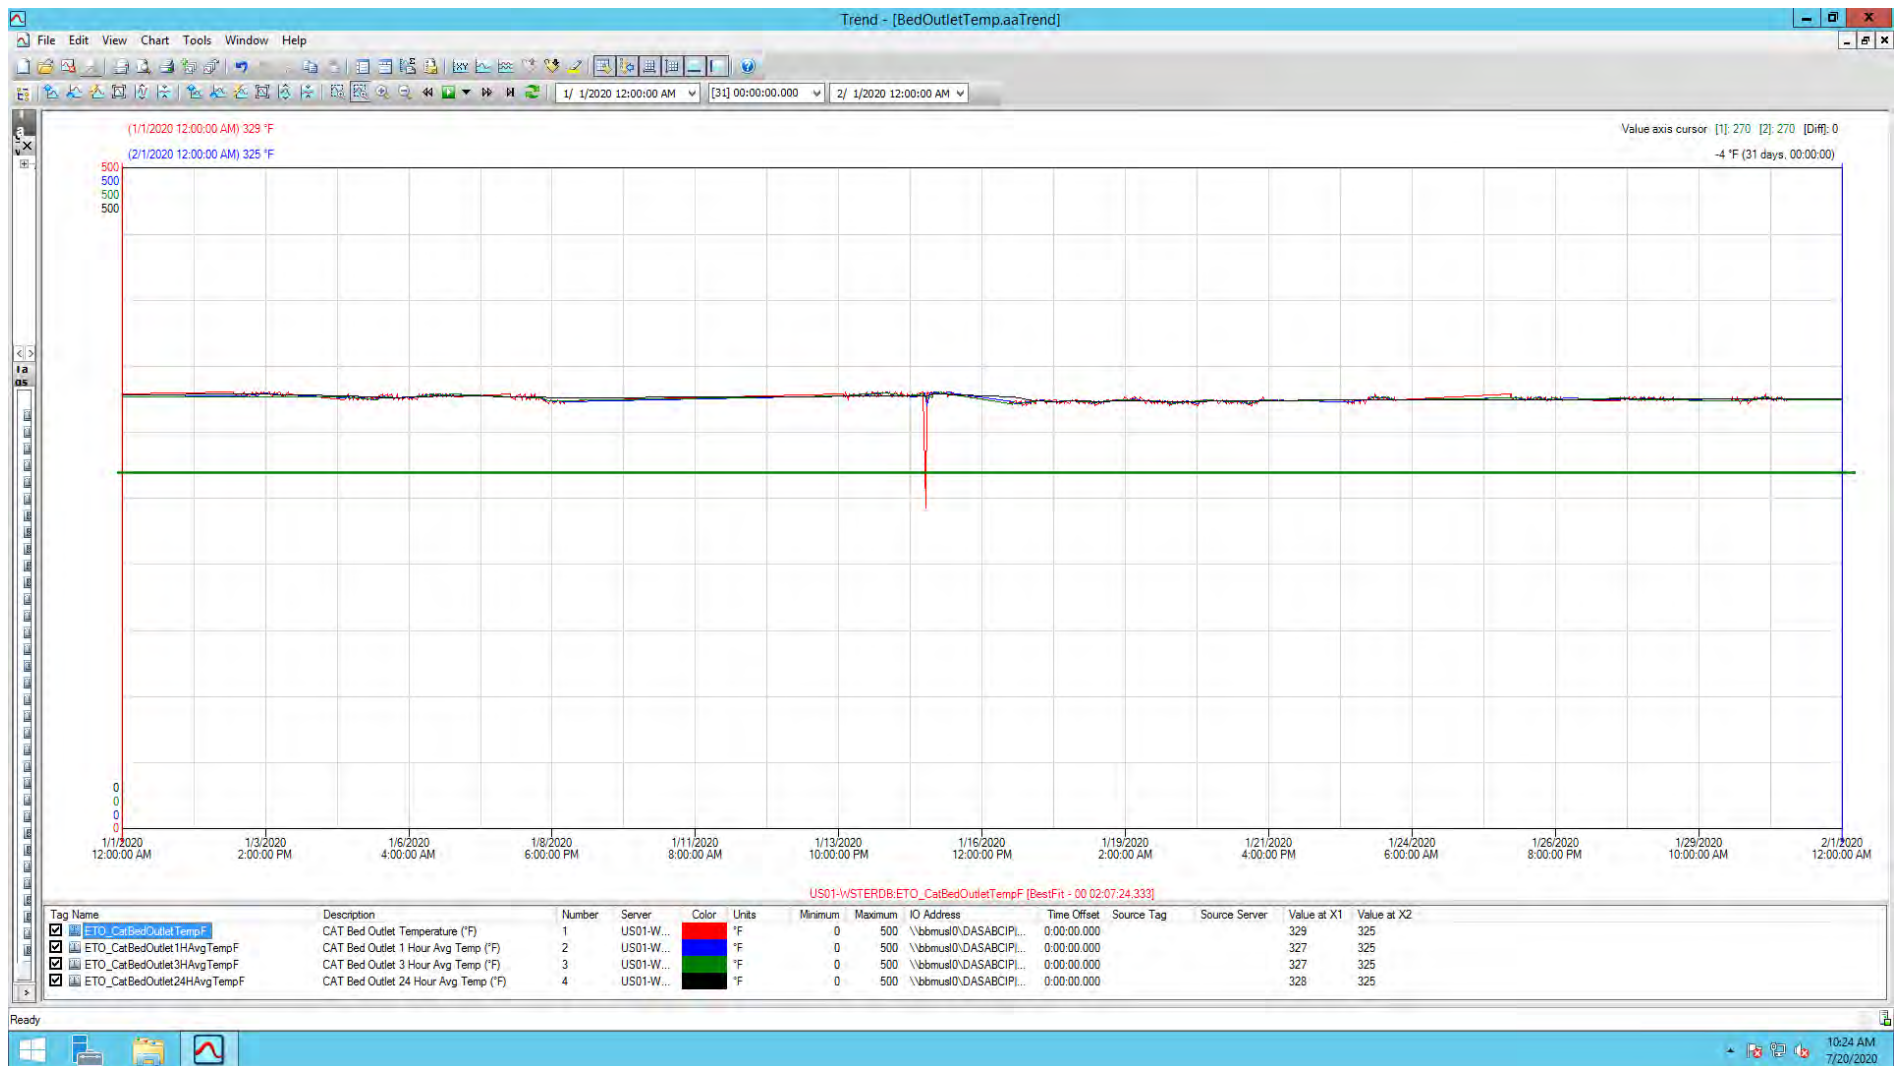


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jan 2020

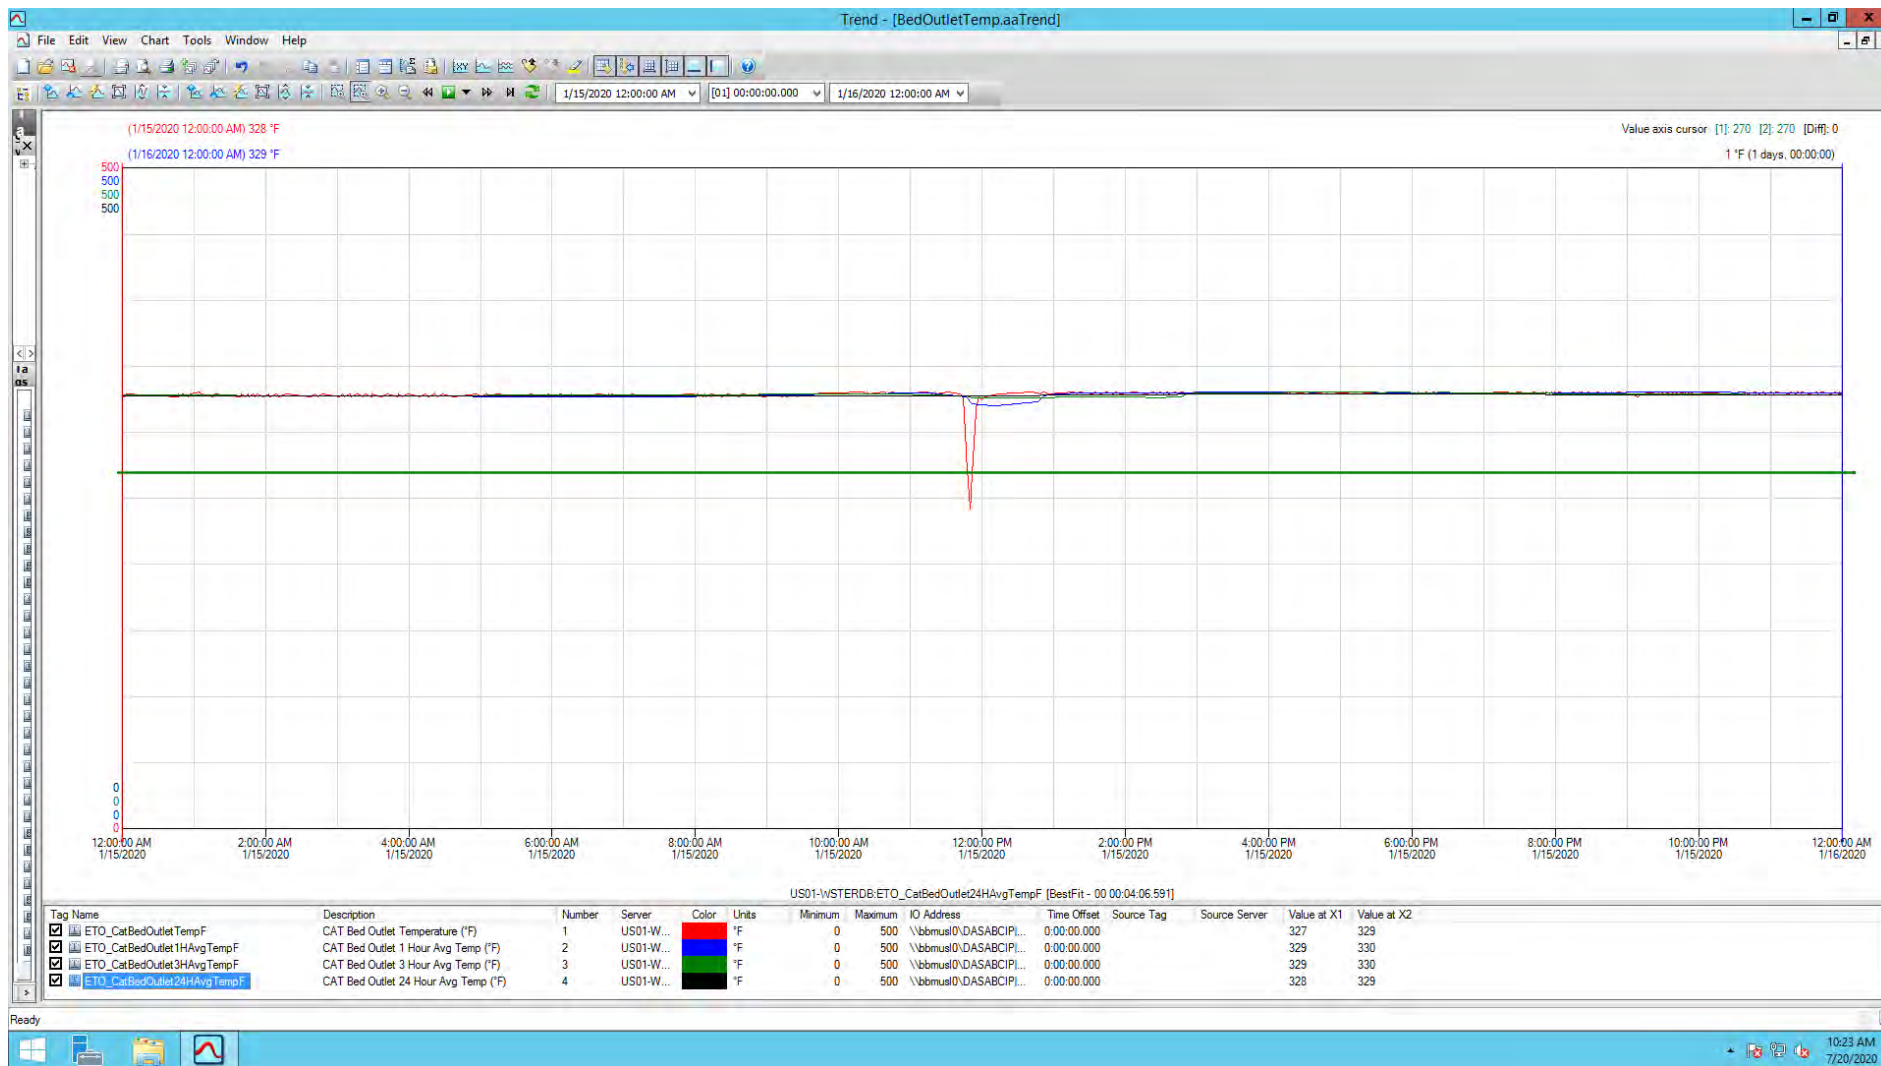

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Feb 2020

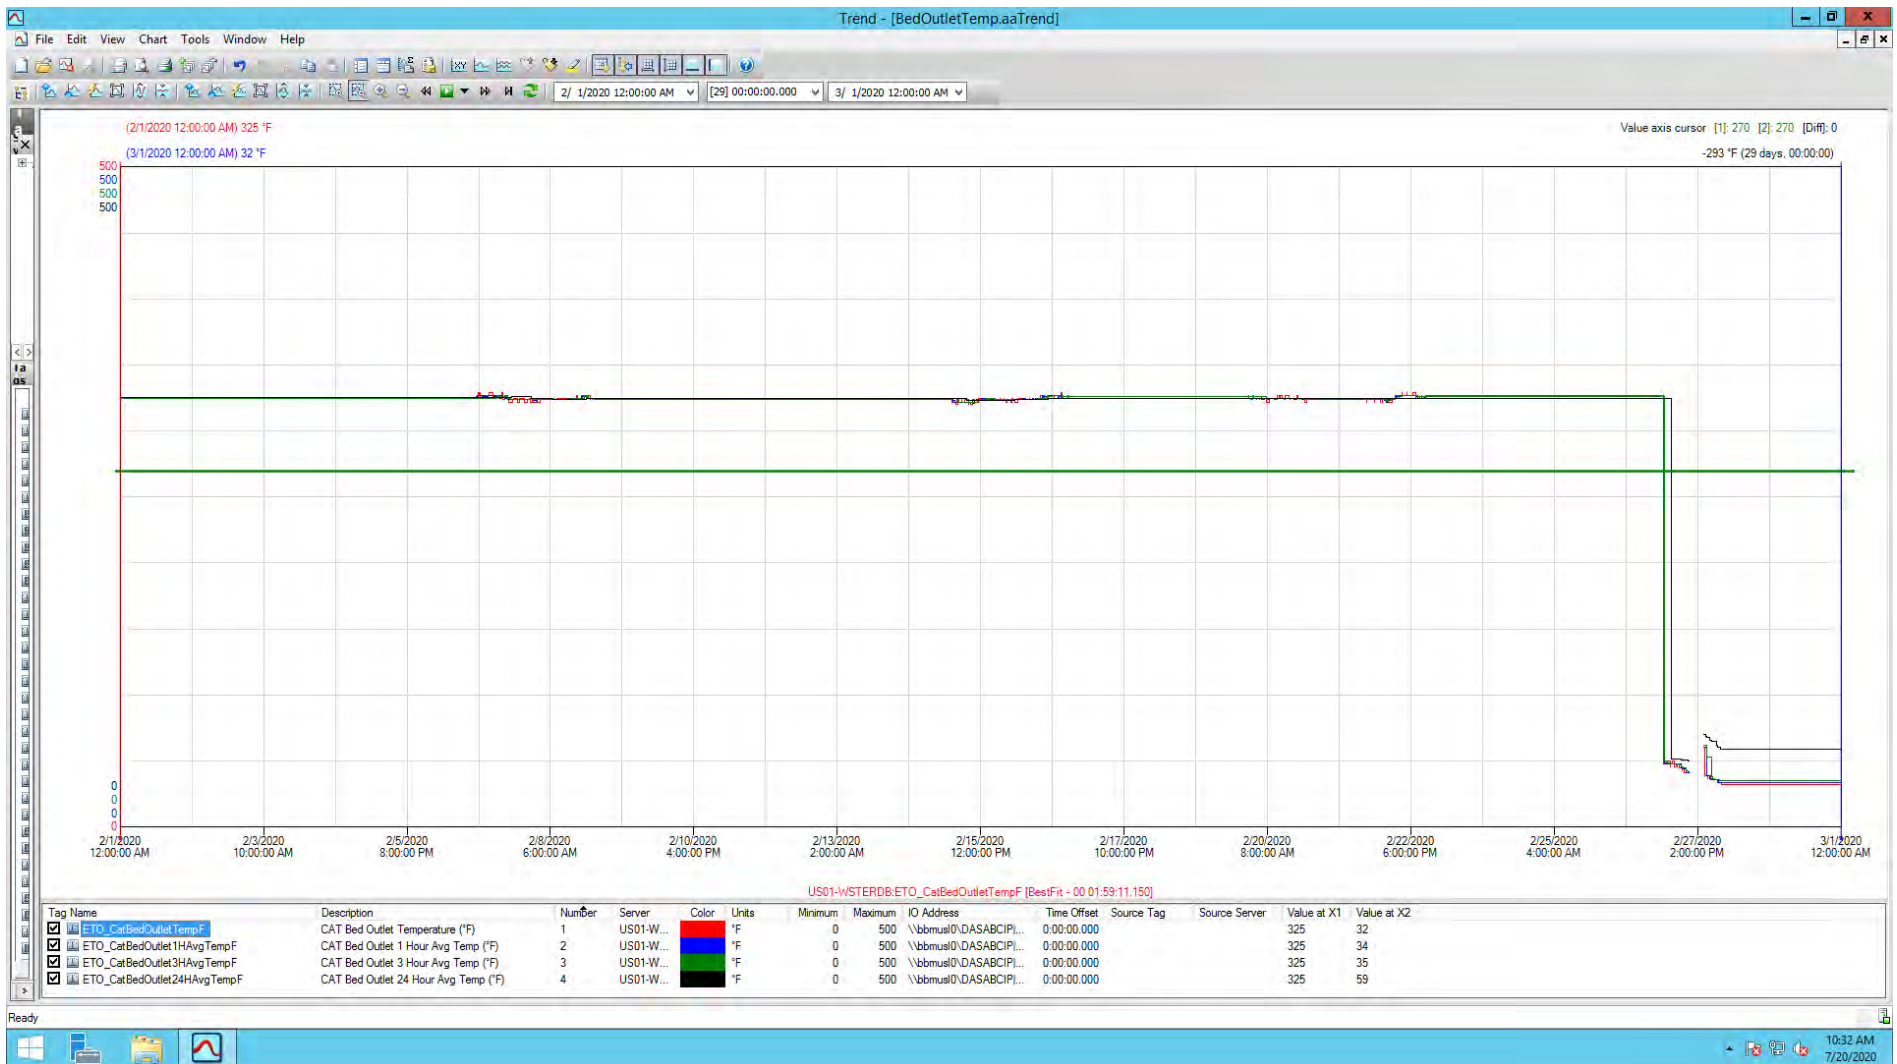


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Mar 2020

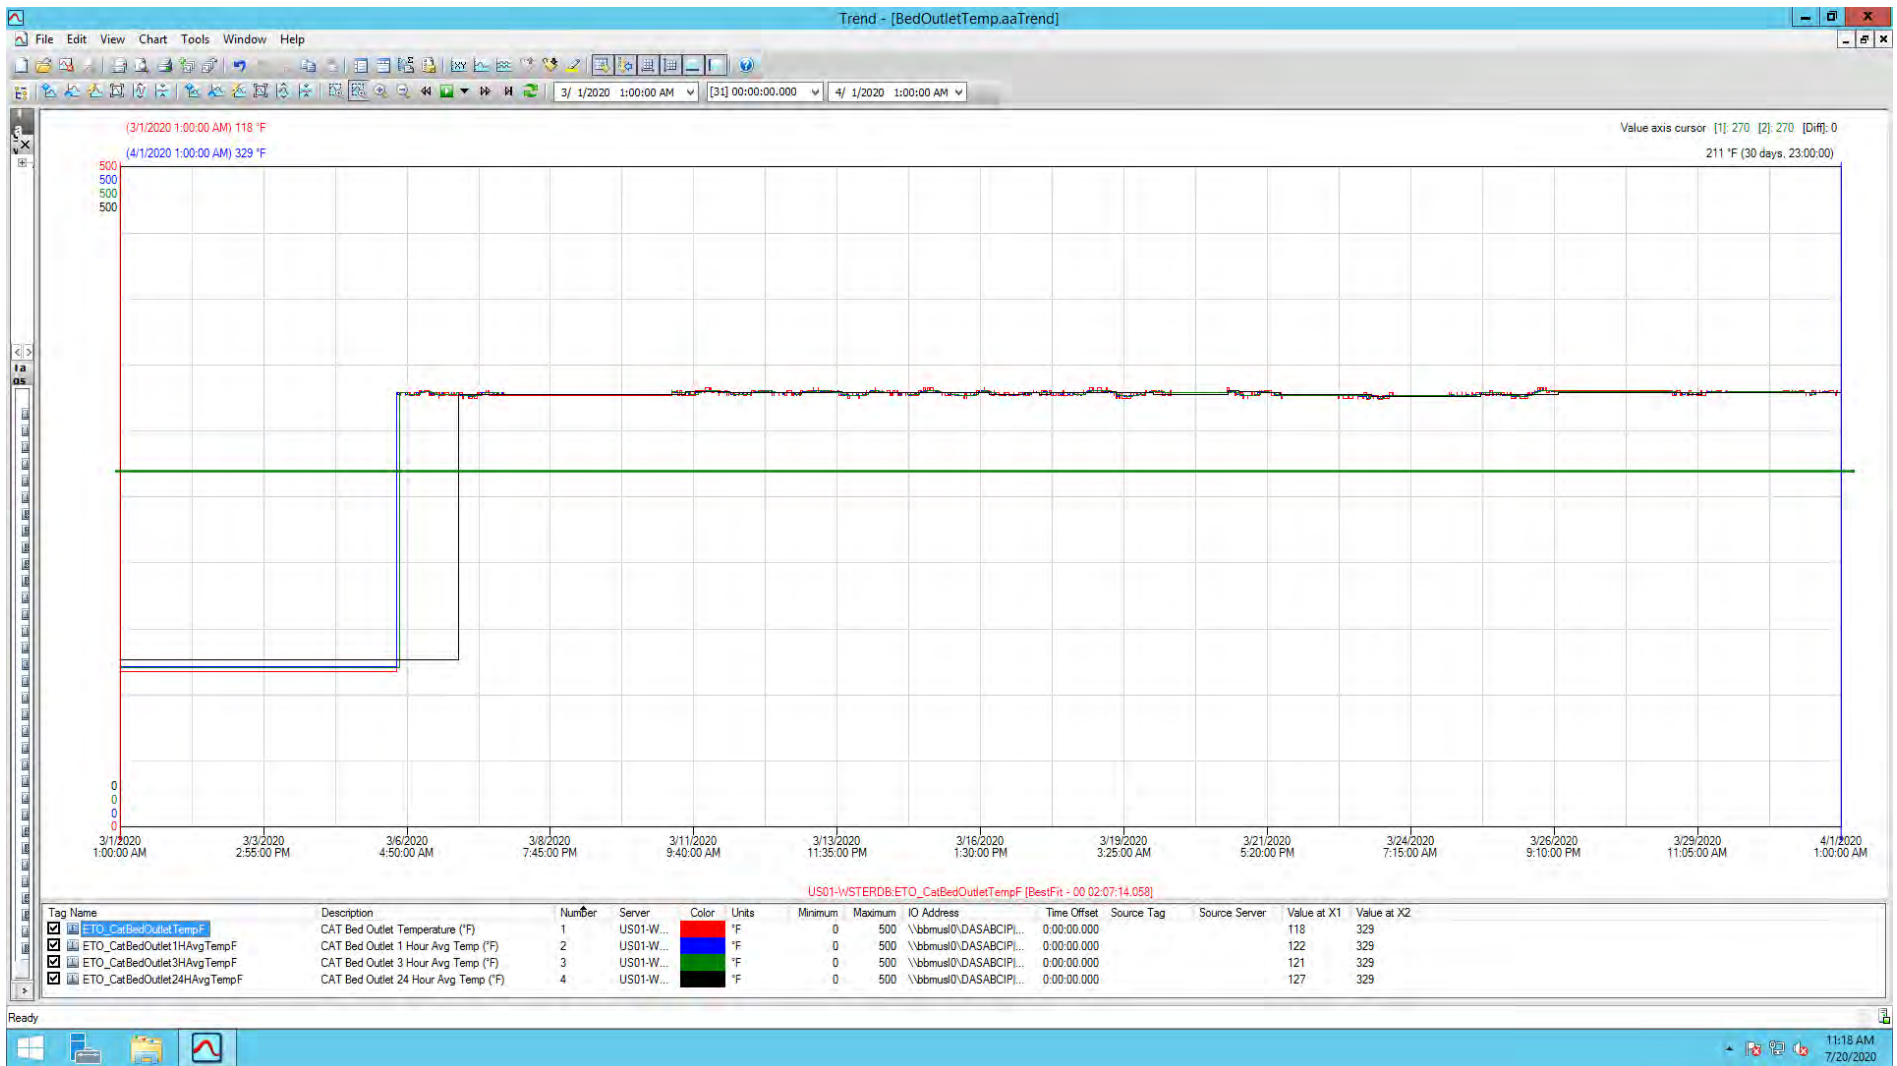





# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Apr 2020

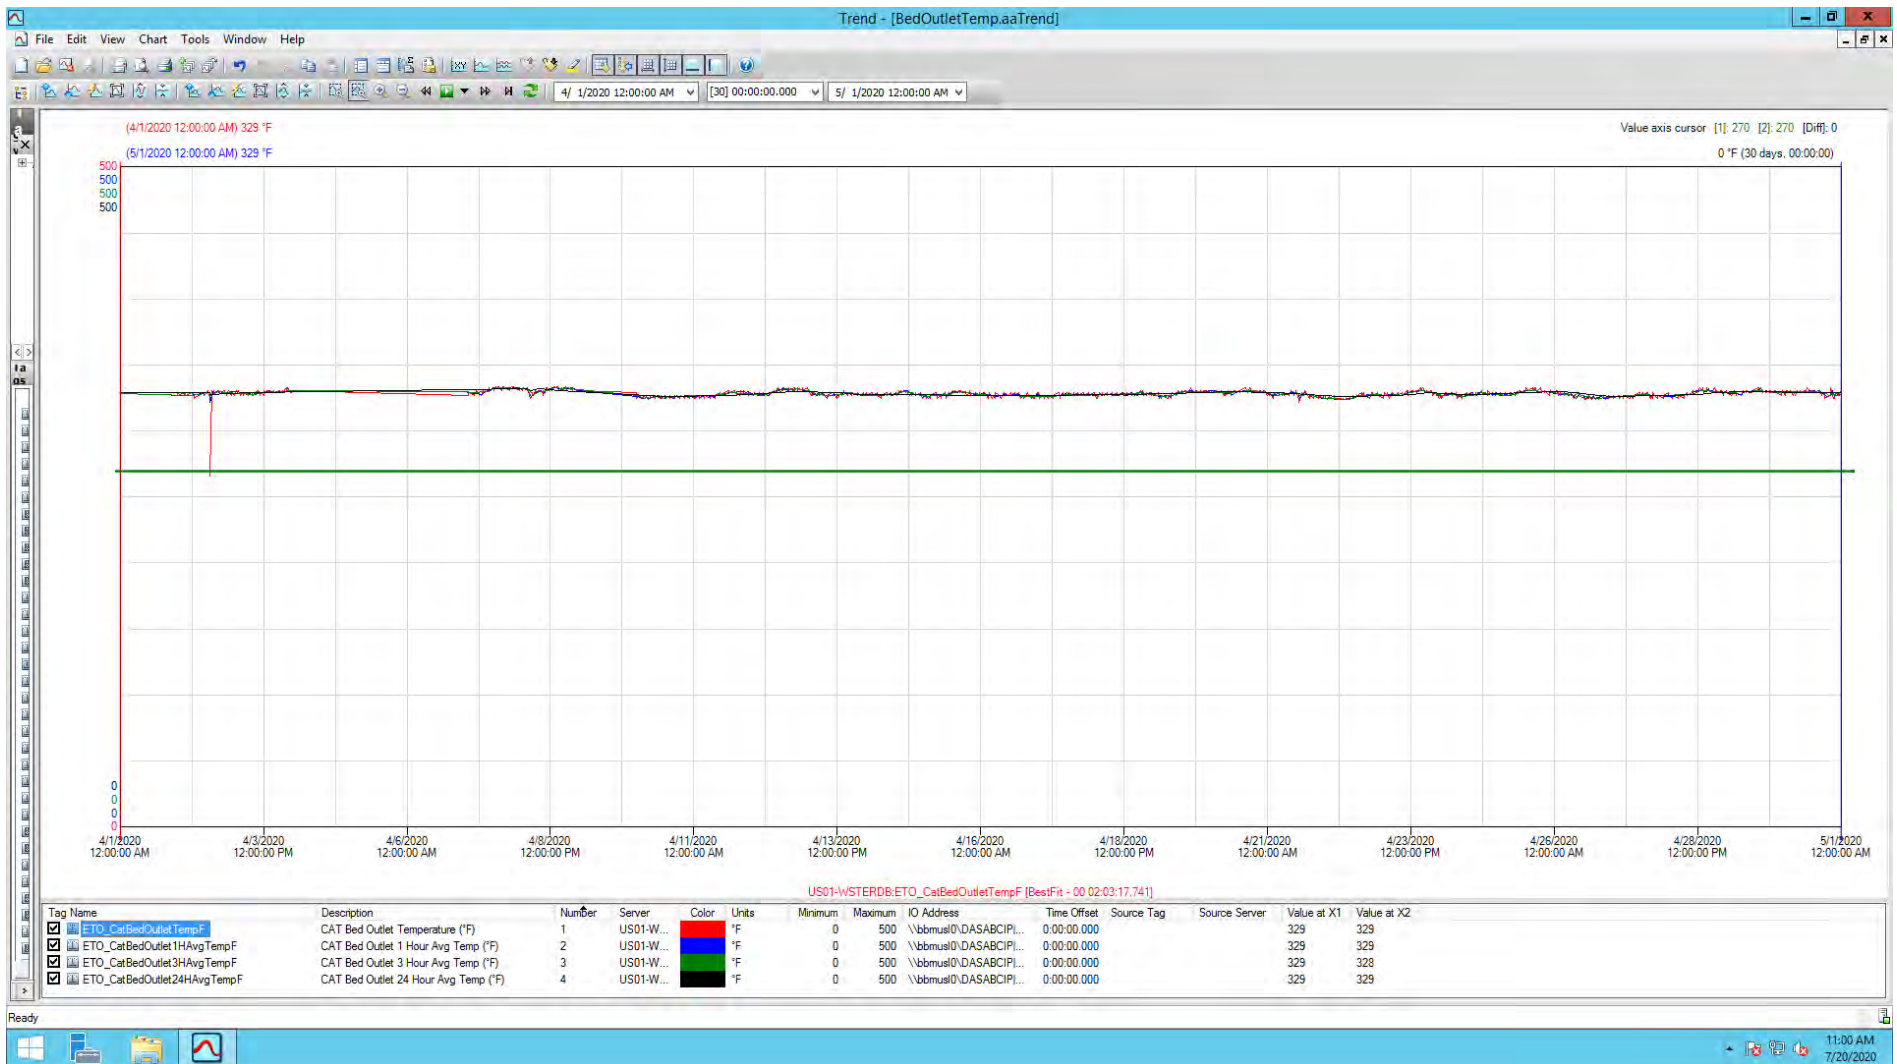


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Apr 2020

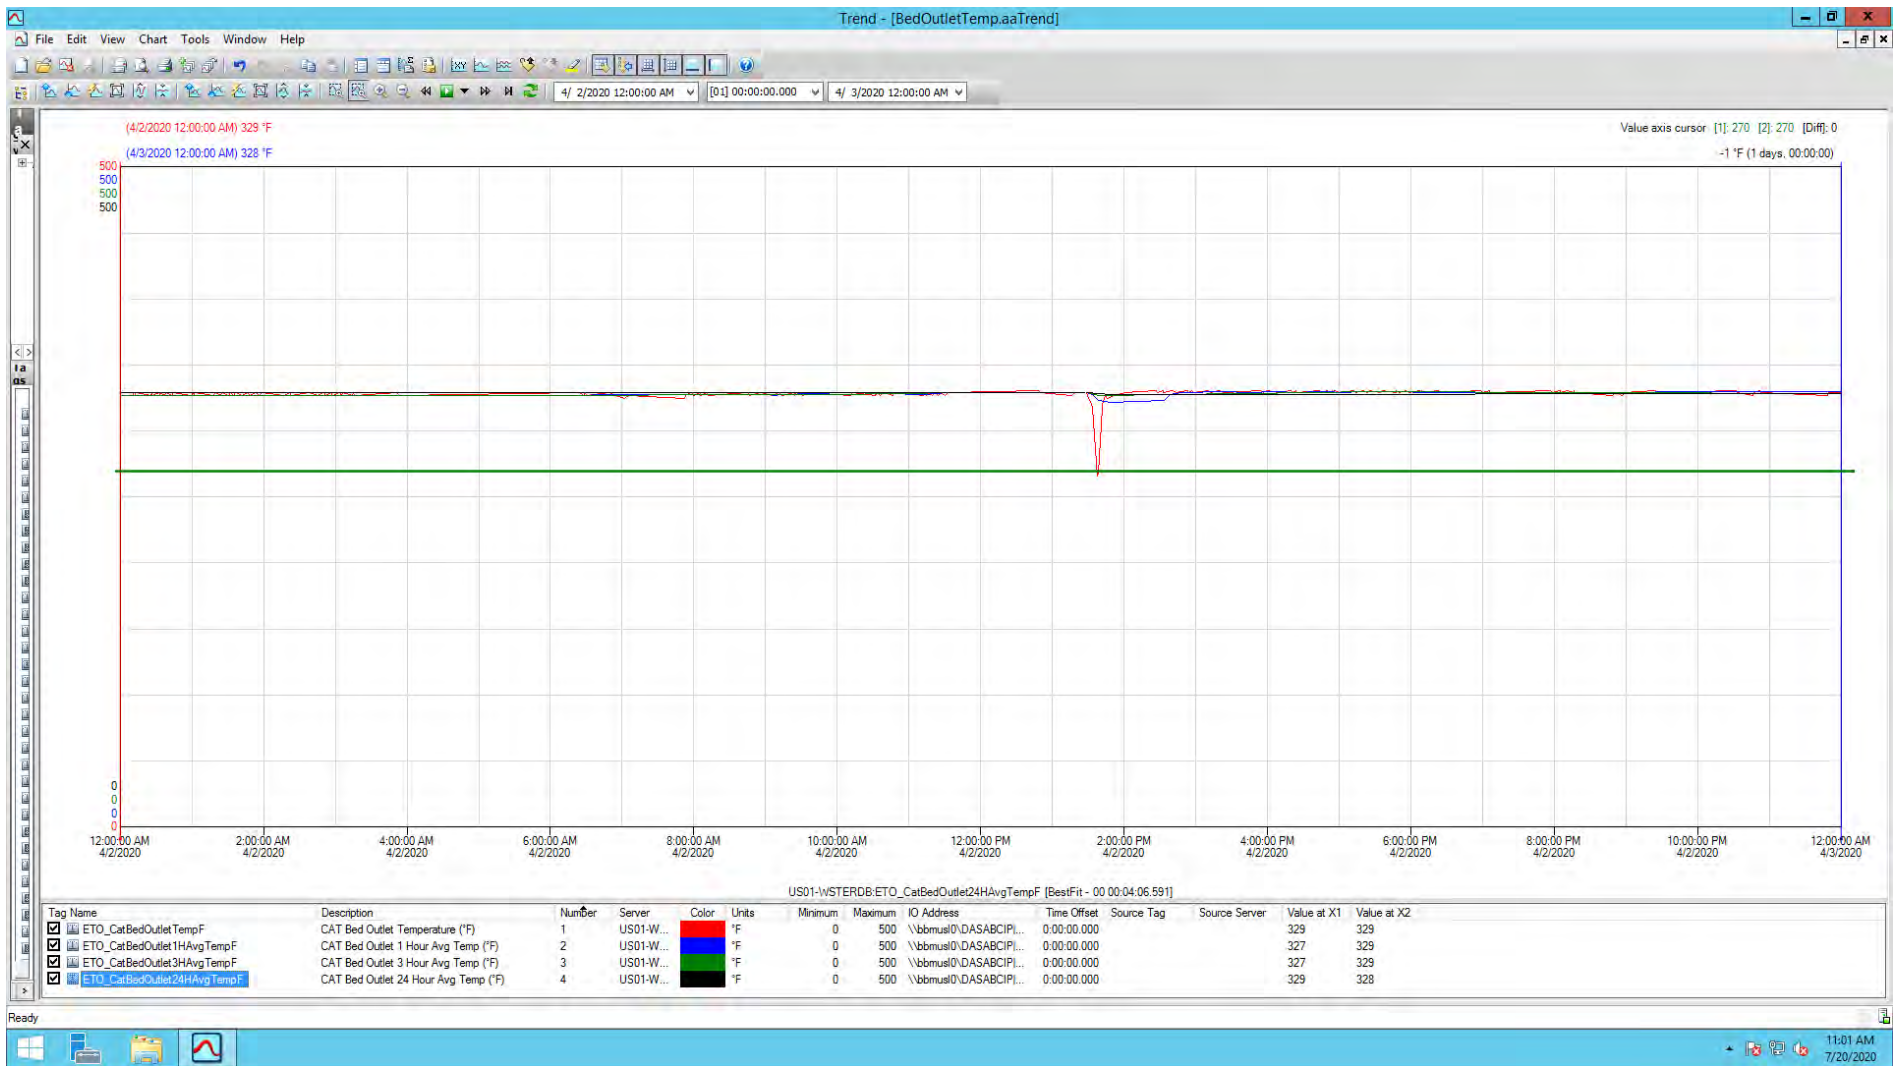

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – May 2020

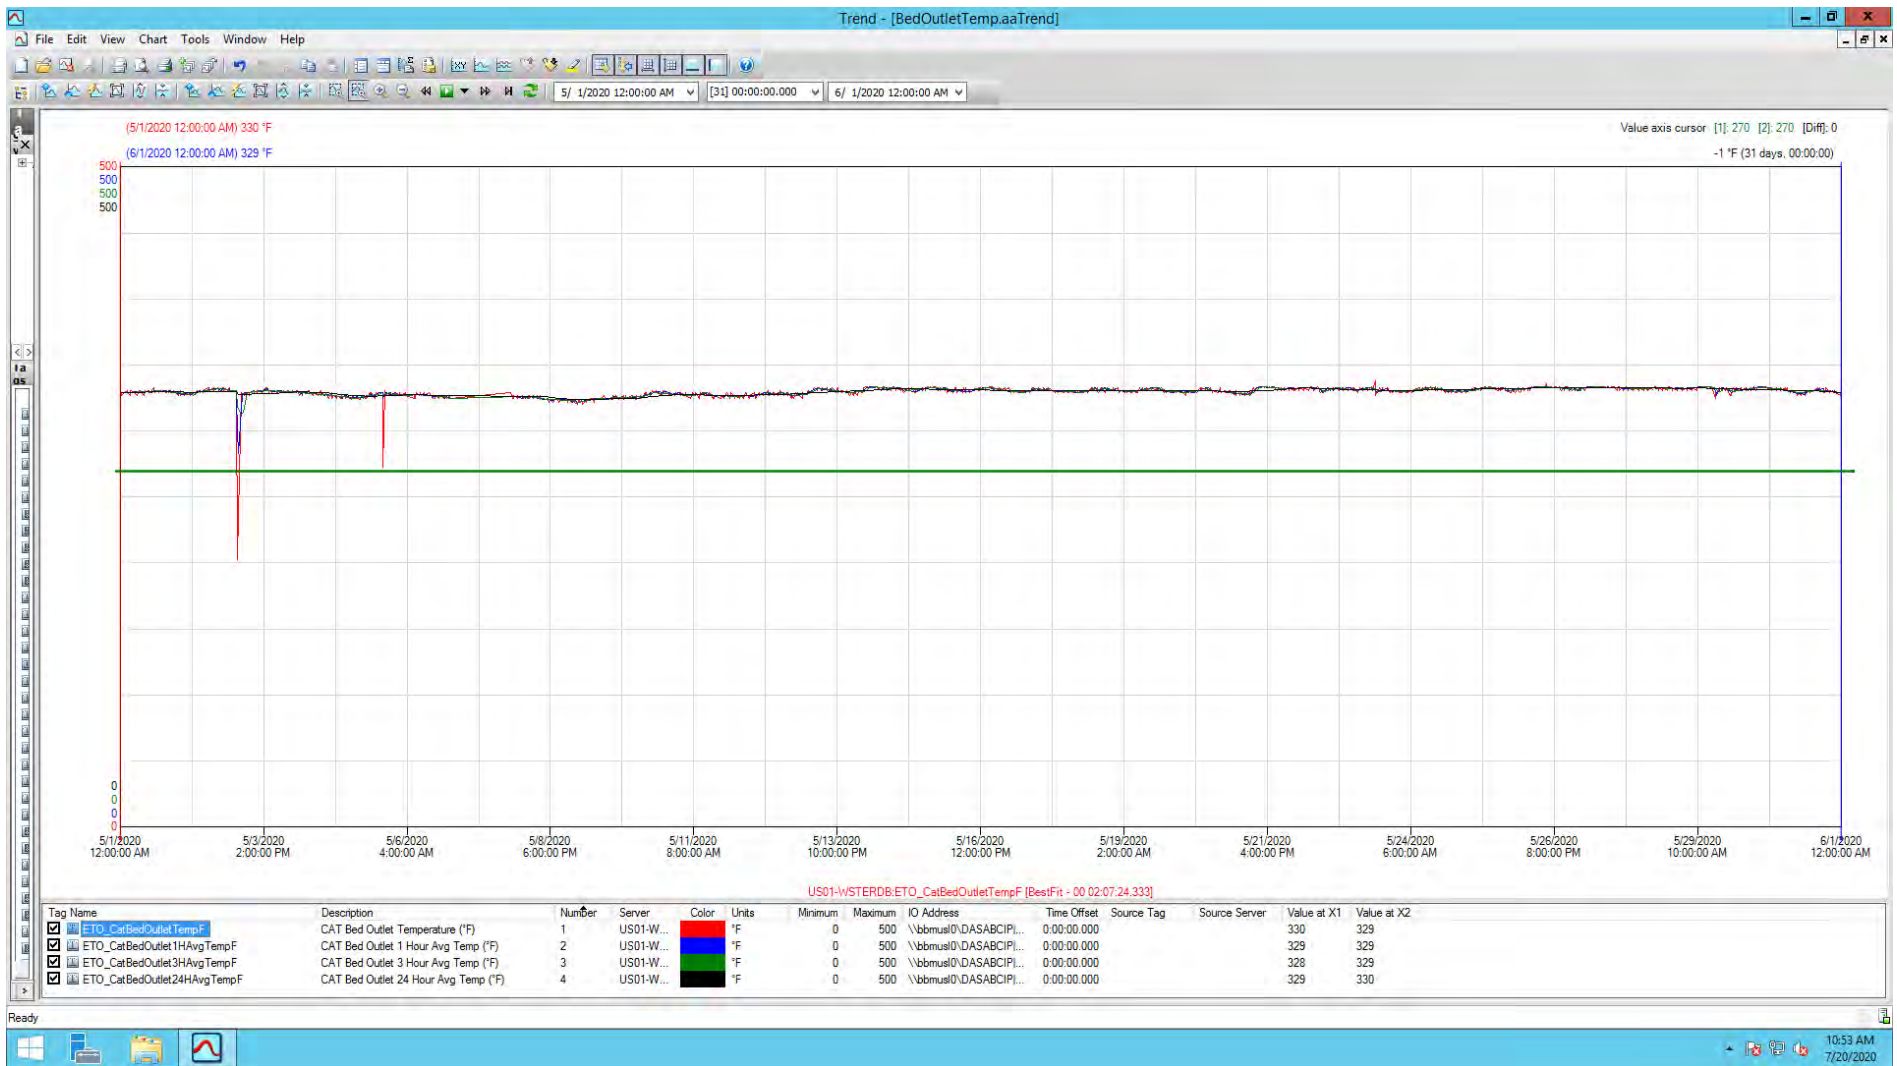


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – May 2020

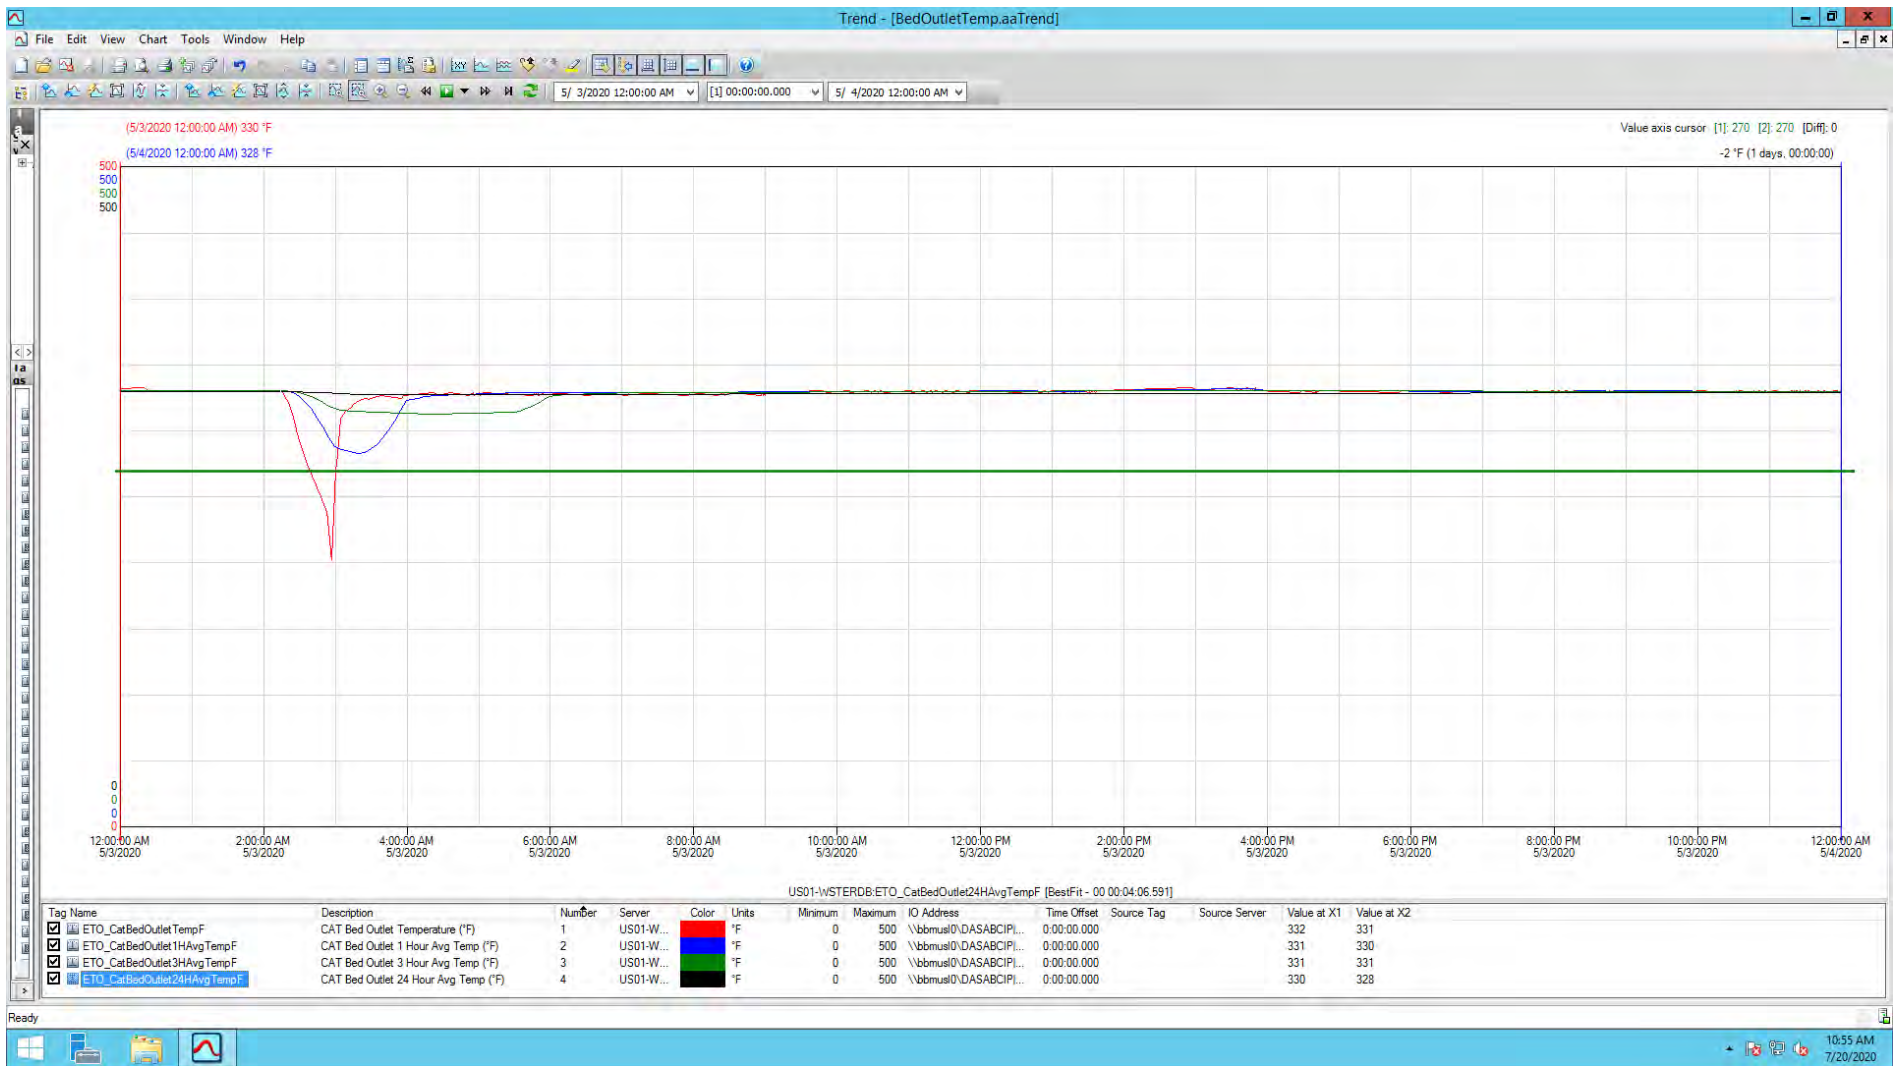




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jun 2020

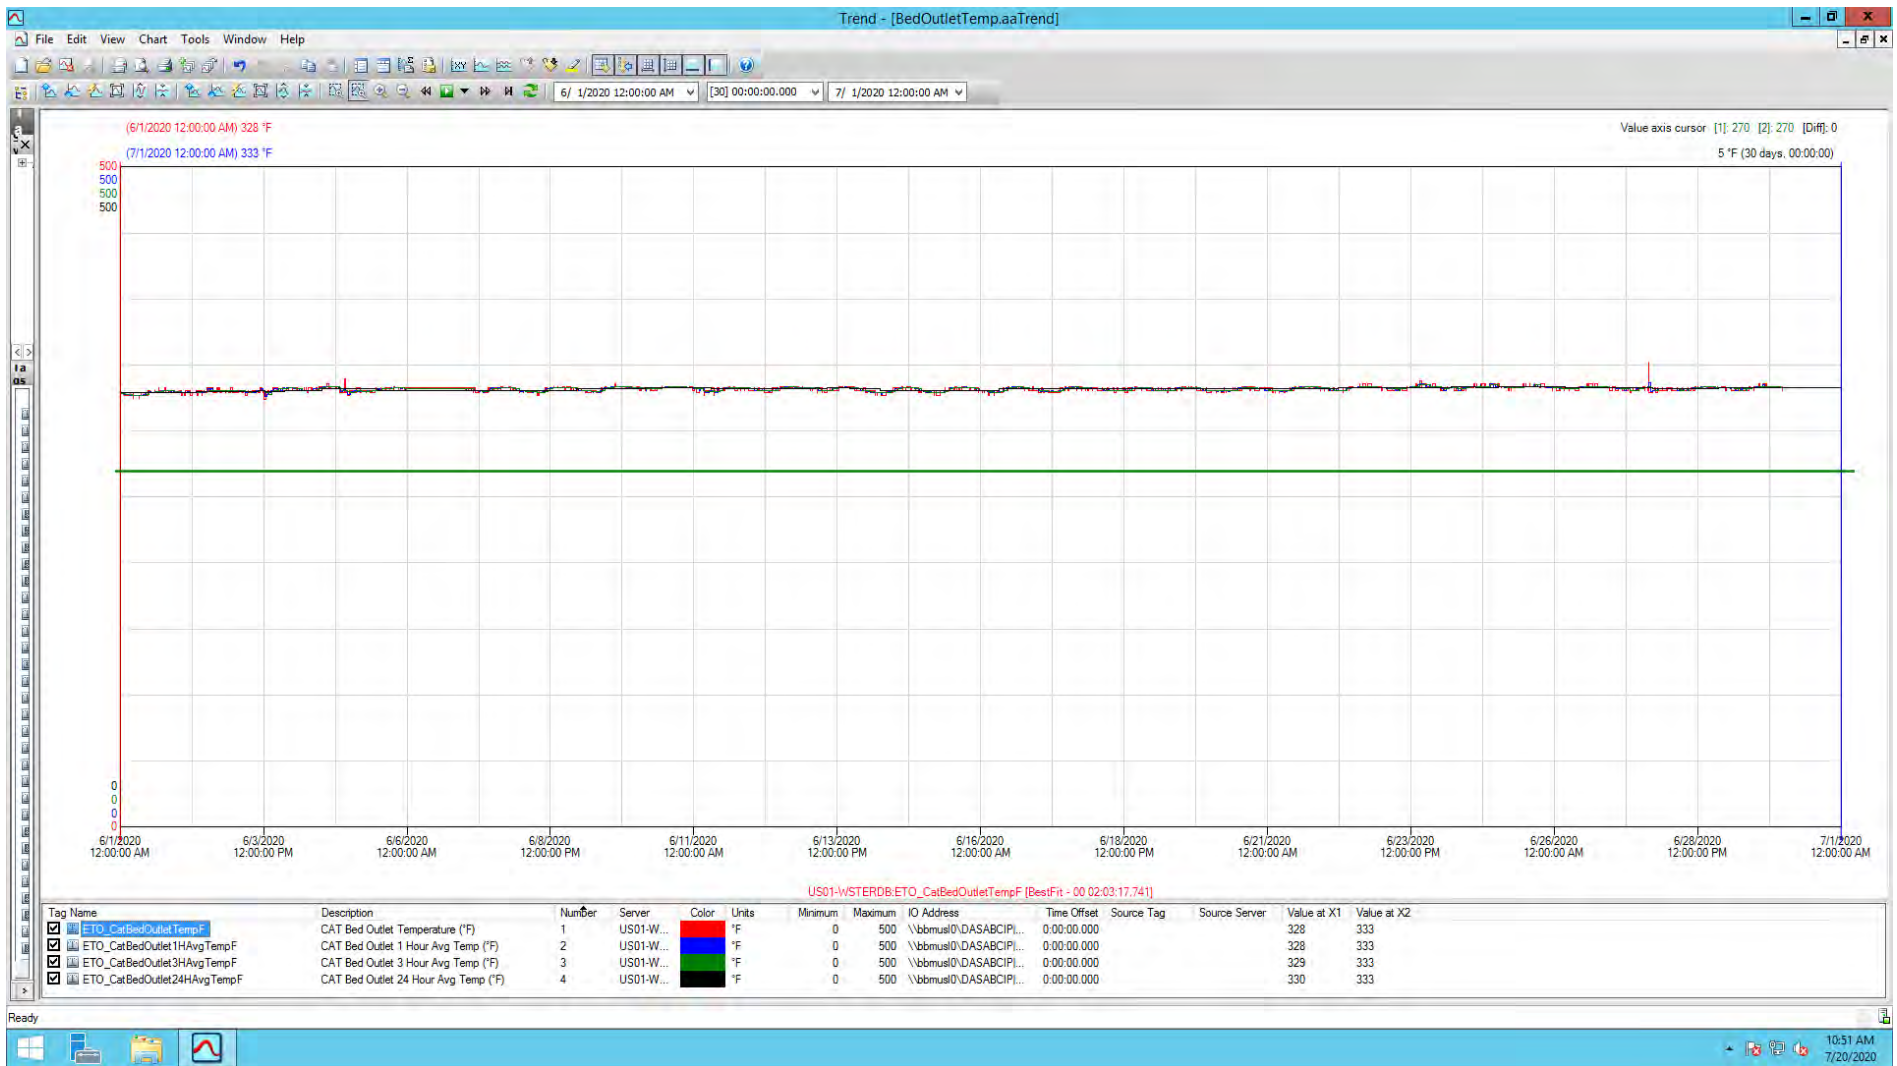


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

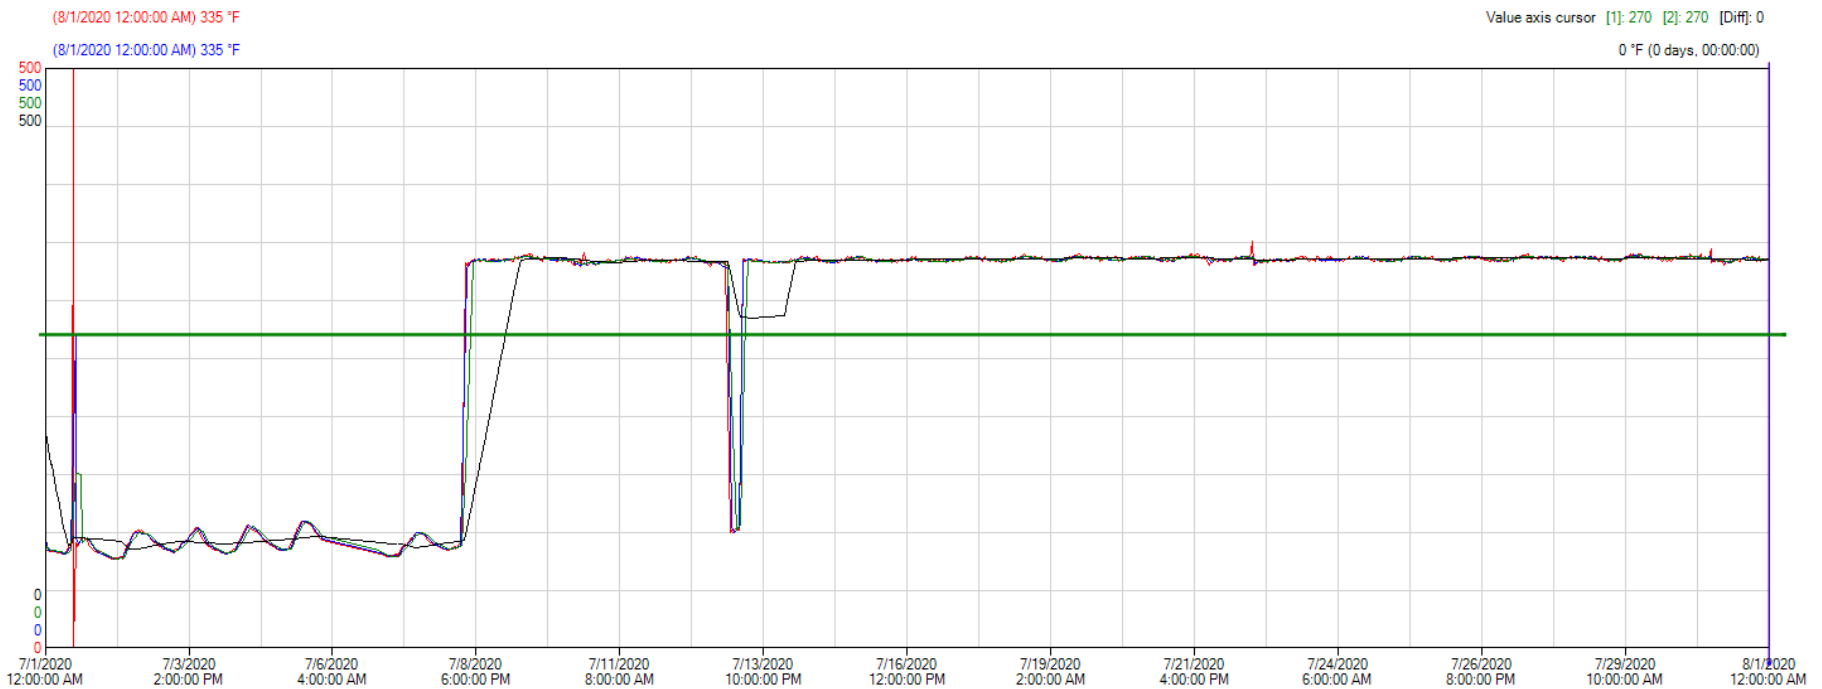


US01-WSTERDB:ETO\_CatBedOutlet24HAvgTempF [BestFit - 00 02:43:09.646]

Tag Name	Description	Number	Server	Color	Units	Minimum	Maximum	IO Address	Time Offset	Source Tag	Source Server	Value at X1	Value at X2
<input checked="" type="checkbox"/> ETO_CatBedOutletTempF	CAT Bed Outlet Temperature (°F)	1	US01-W...	Red	°F	0	500	\\bbmusl0\ DASABCI\ETO_1Sec\N27:420	0:00:00.000			336	336
<input checked="" type="checkbox"/> ETO_CatBedOutlet1HAvgTempF	CAT Bed Outlet 1 Hour Avg Temp (°F)	2	US01-W...	Blue	°F	0	500	\\bbmusl0\ DASABCI\ETO_1Sec\N27:650	0:00:00.000			336	336
<input checked="" type="checkbox"/> ETO_CatBedOutlet3HAvgTempF	CAT Bed Outlet 3 Hour Avg Temp (°F)	3	US01-W...	Green	°F	0	500	\\bbmusl0\ DASABCI\ETO_1Sec\N27:670	0:00:00.000			336	336
<input checked="" type="checkbox"/> ETO_CatBedOutlet24HAvgTempF	CAT Bed Outlet 24 Hour Avg Temp (°F)	4	US01-W...	Black	°F	0	500	\\bbmusl0\ DASABCI\ETO_1Sec\N27:710	0:00:00.000			335	335

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

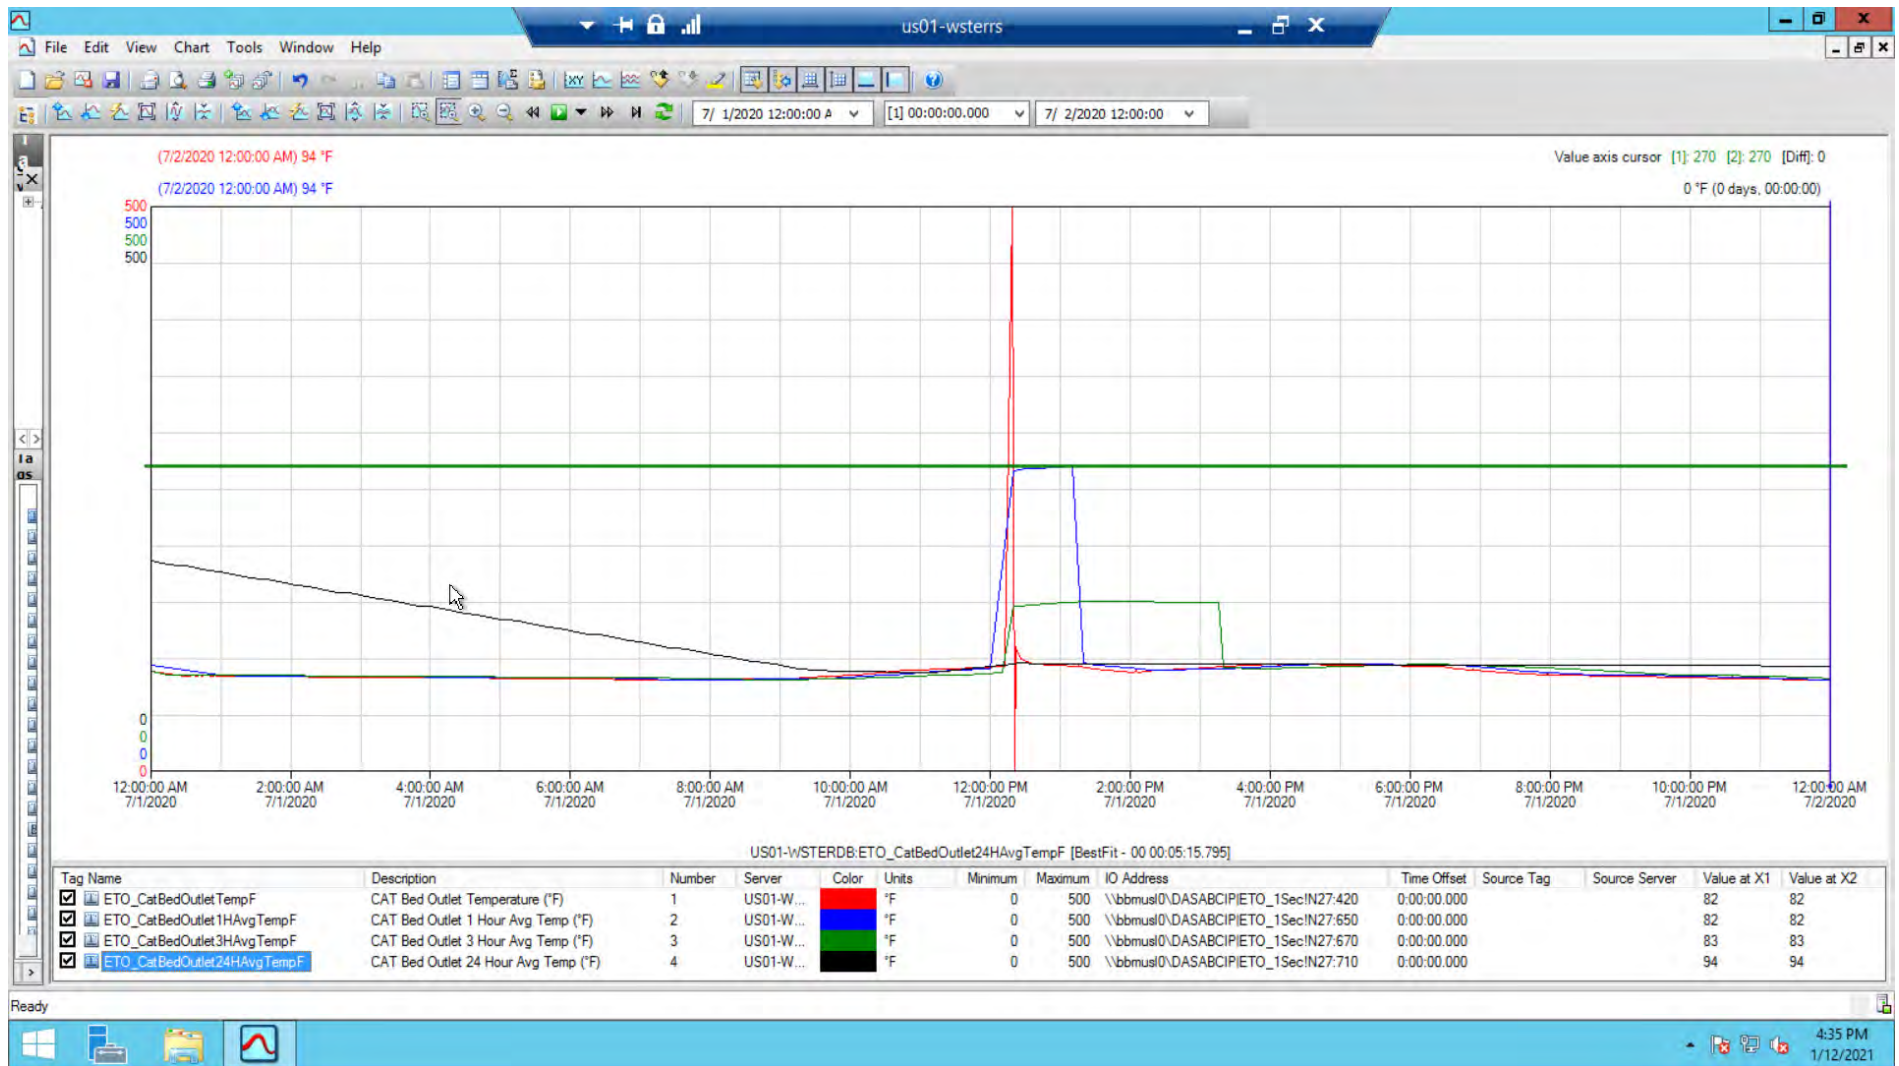


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

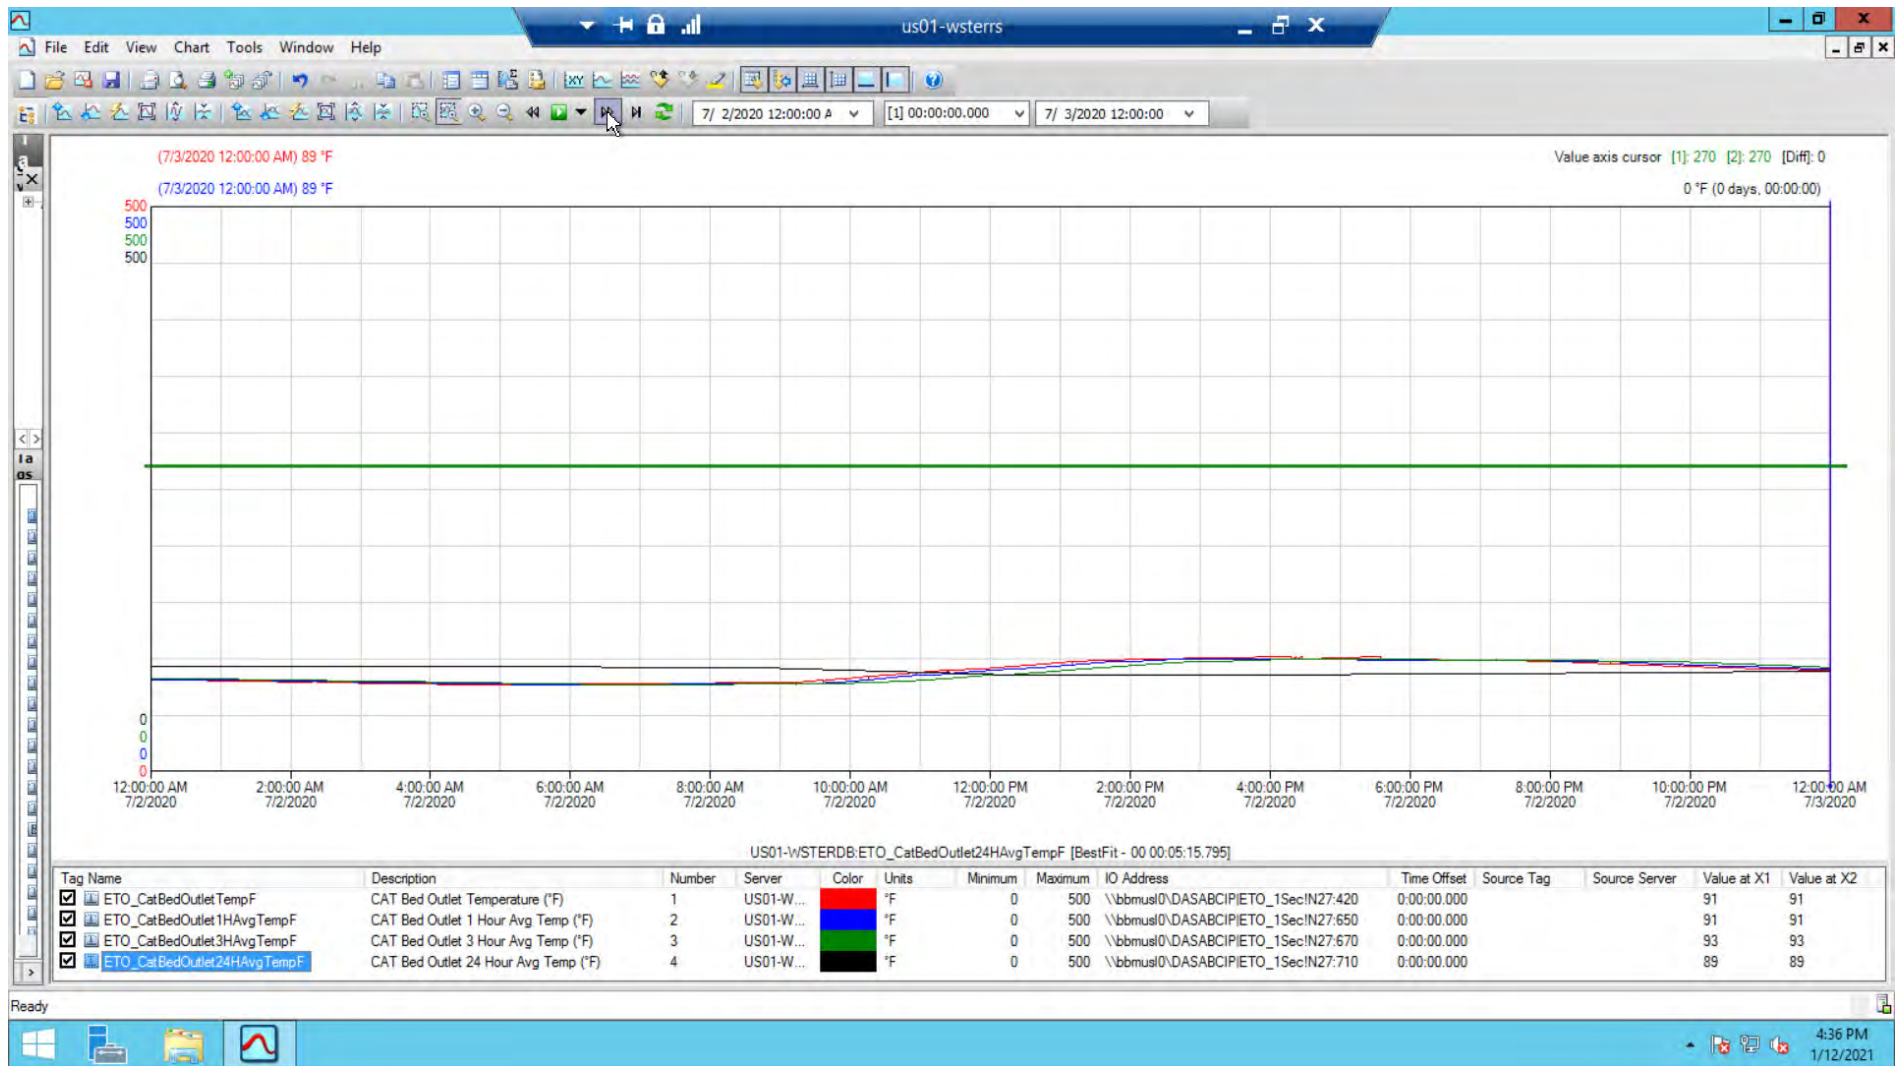





# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

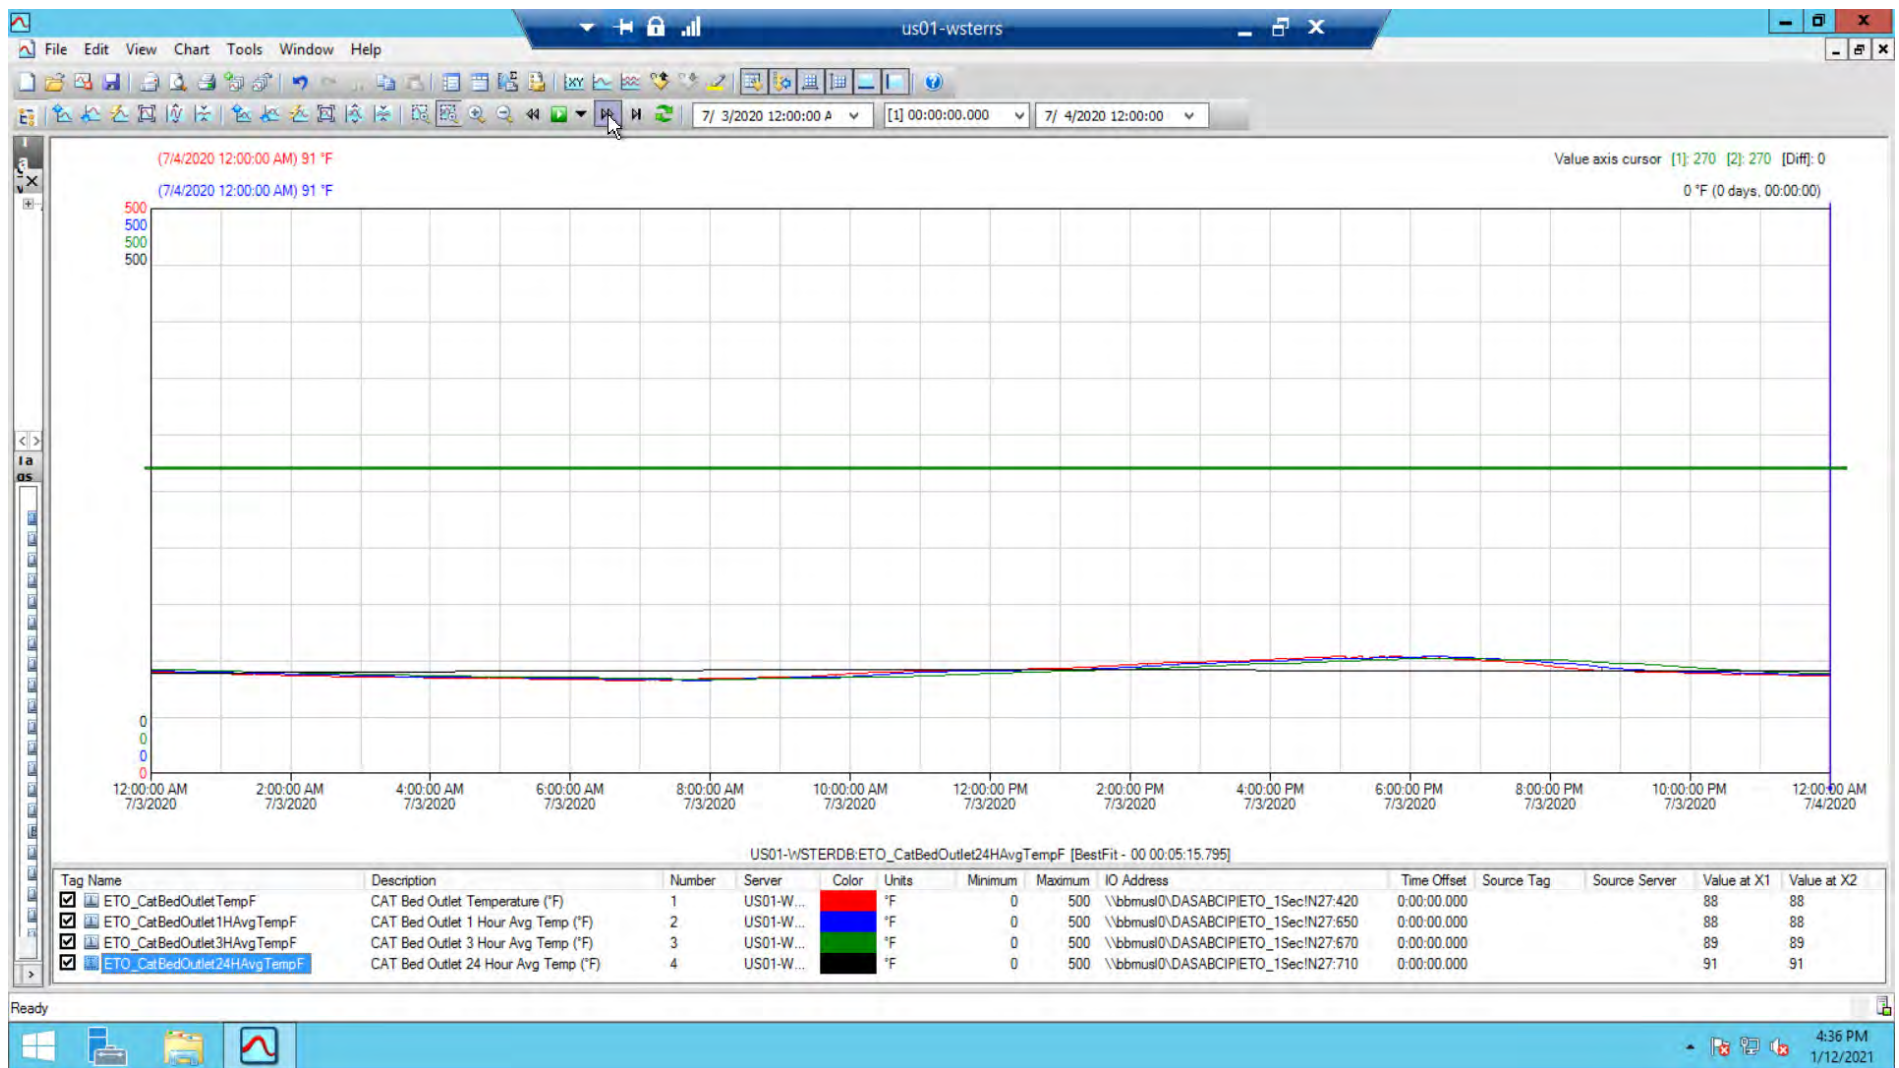

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

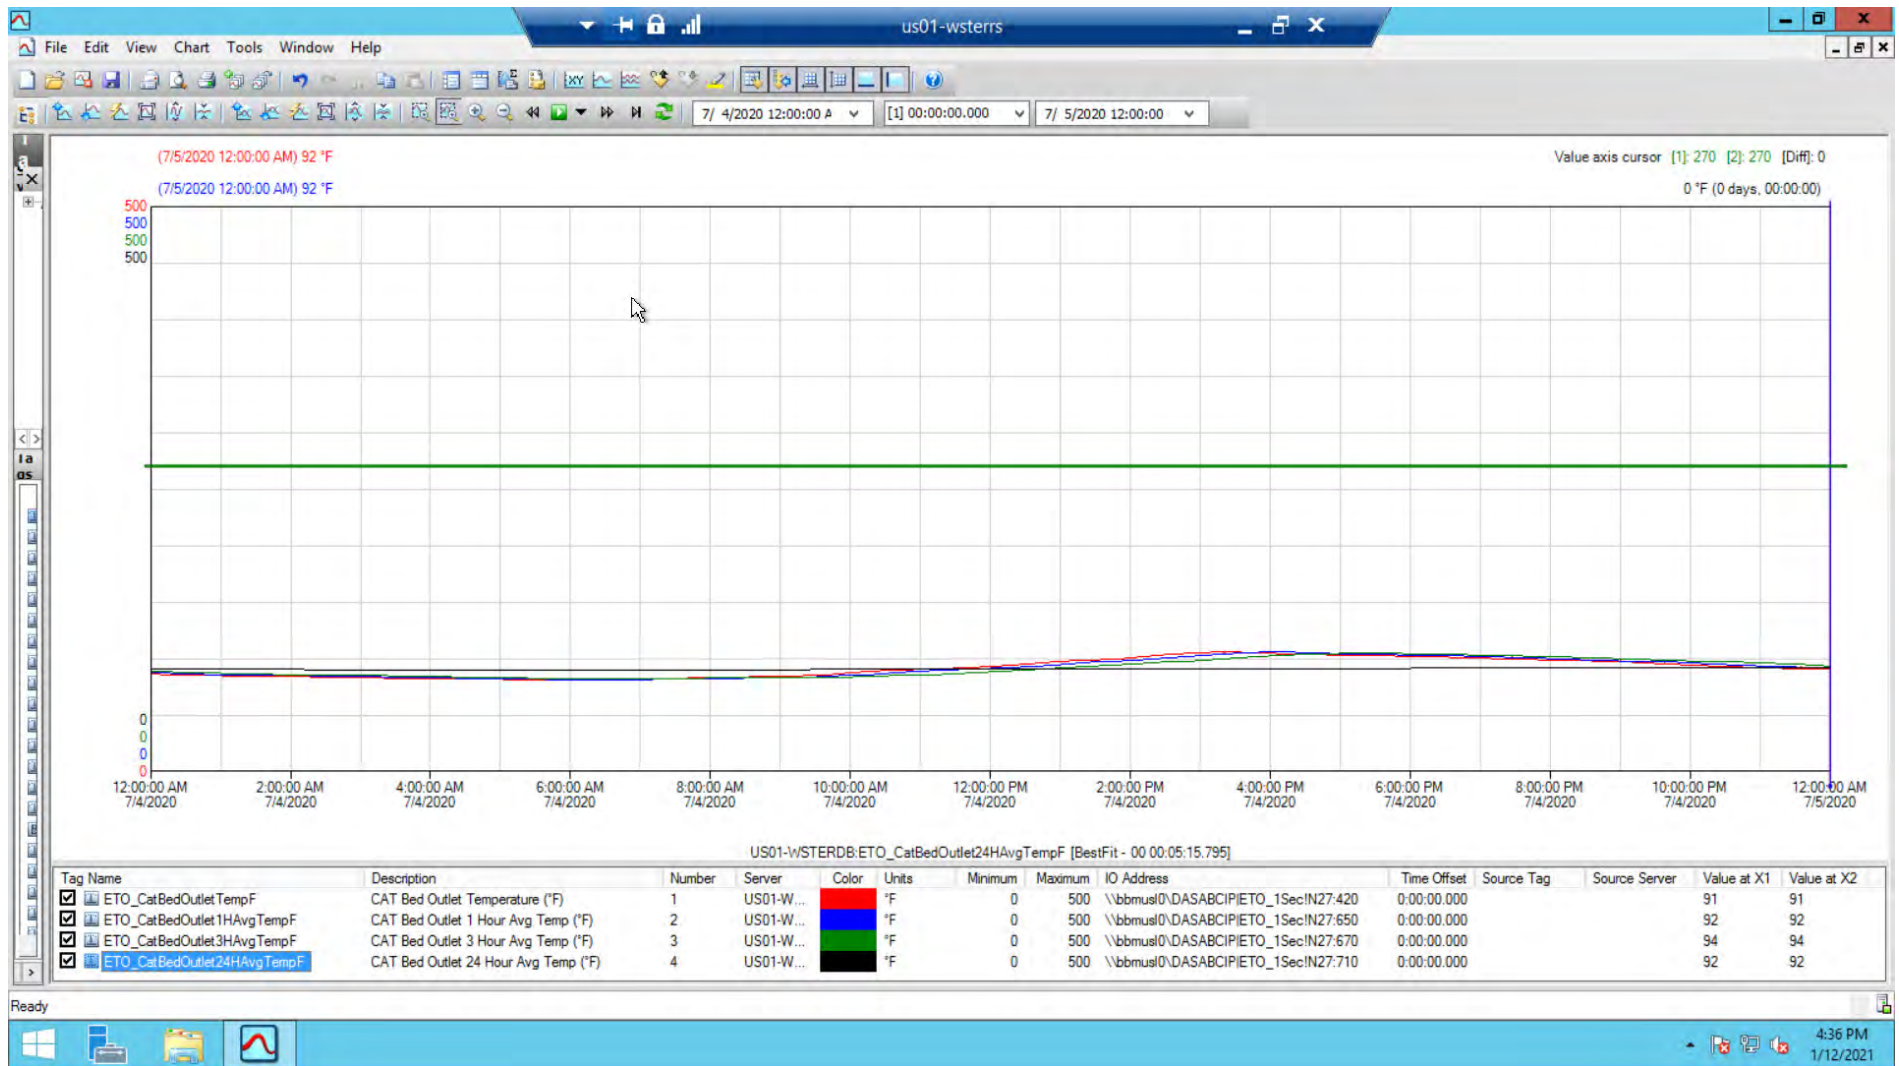


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

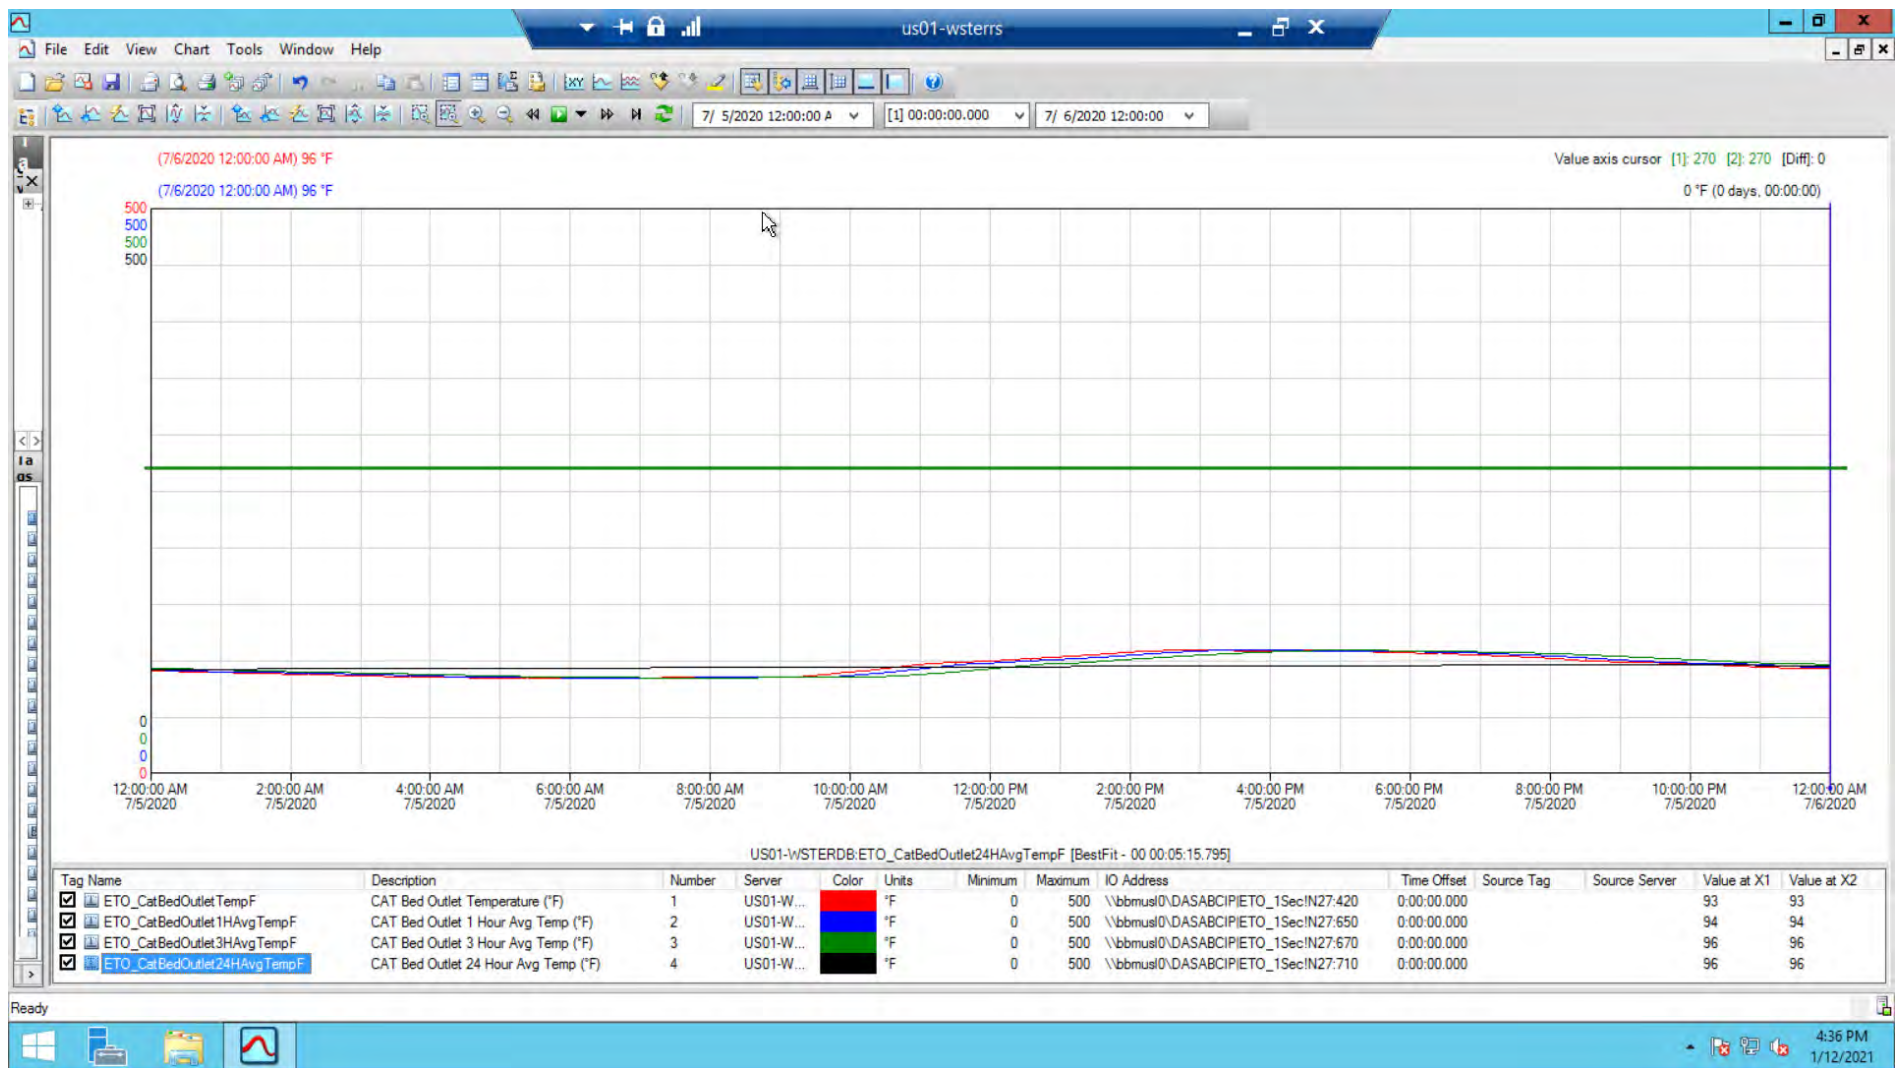




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

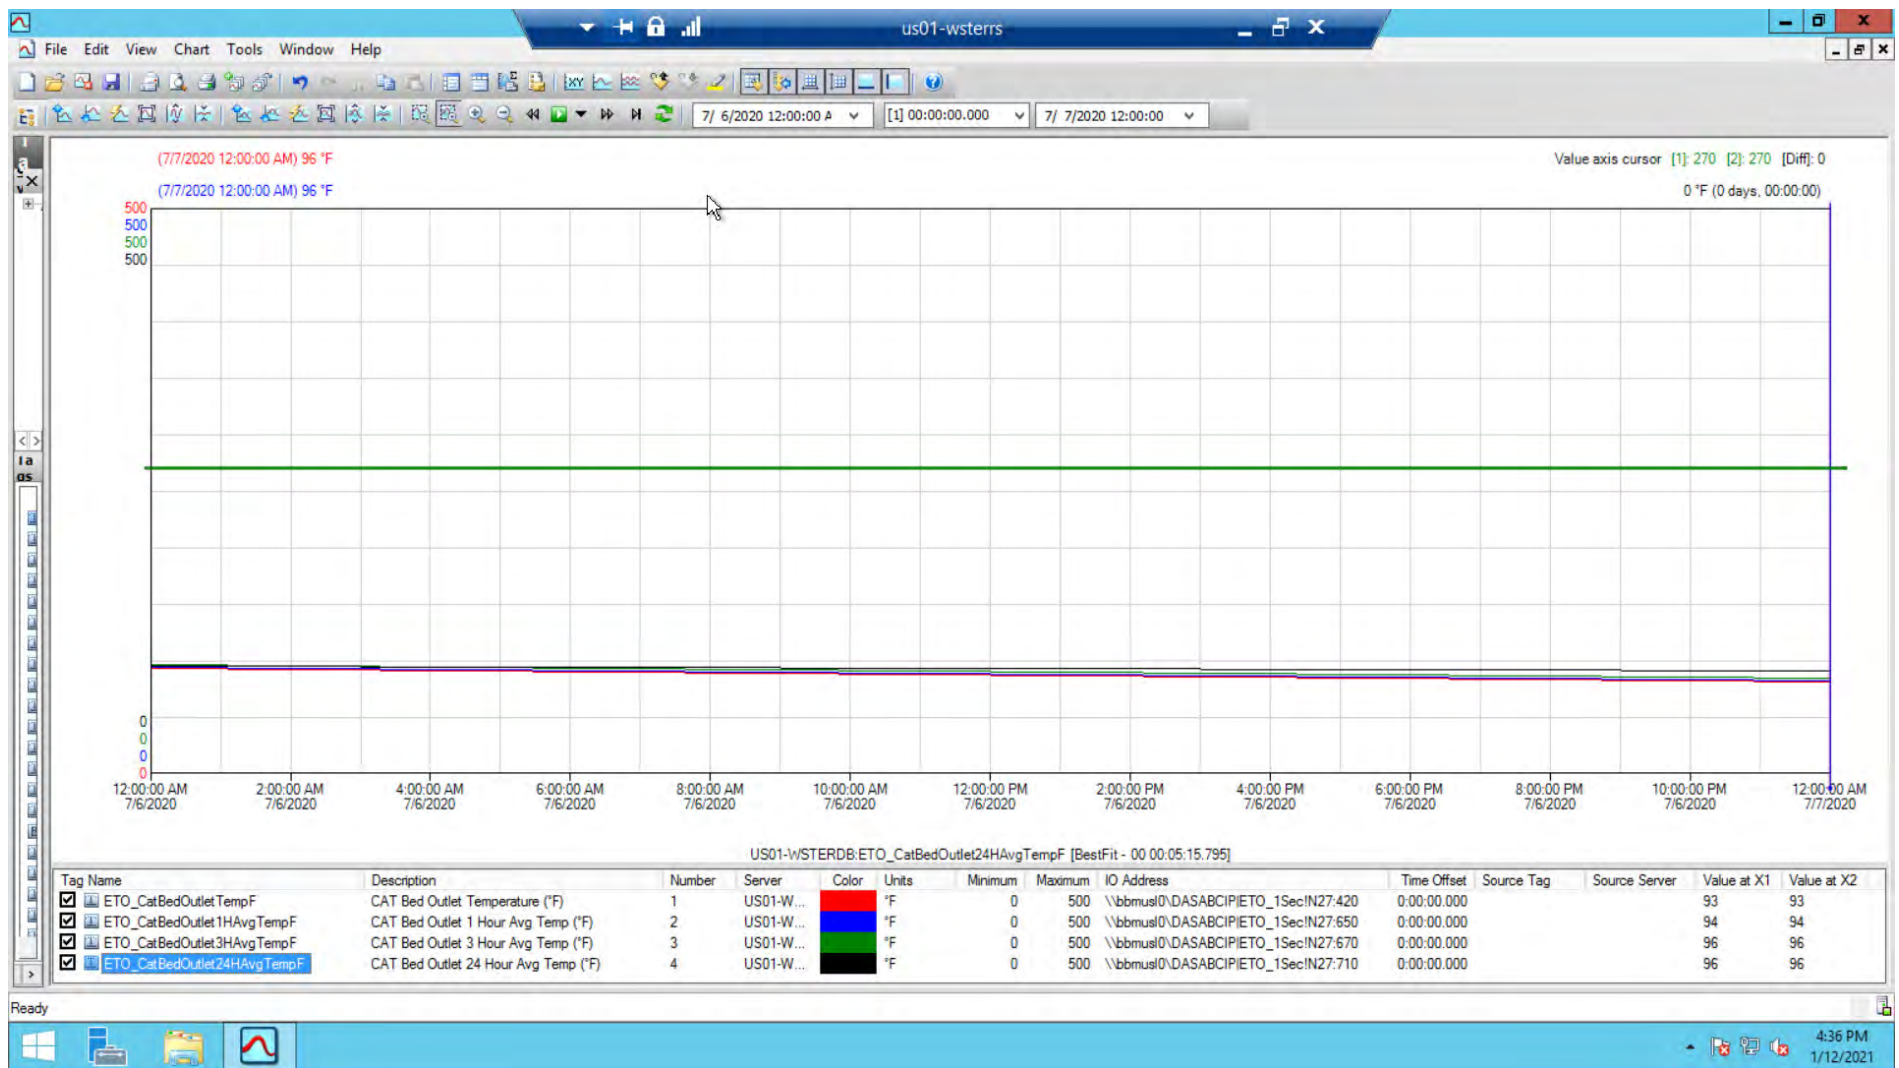





# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

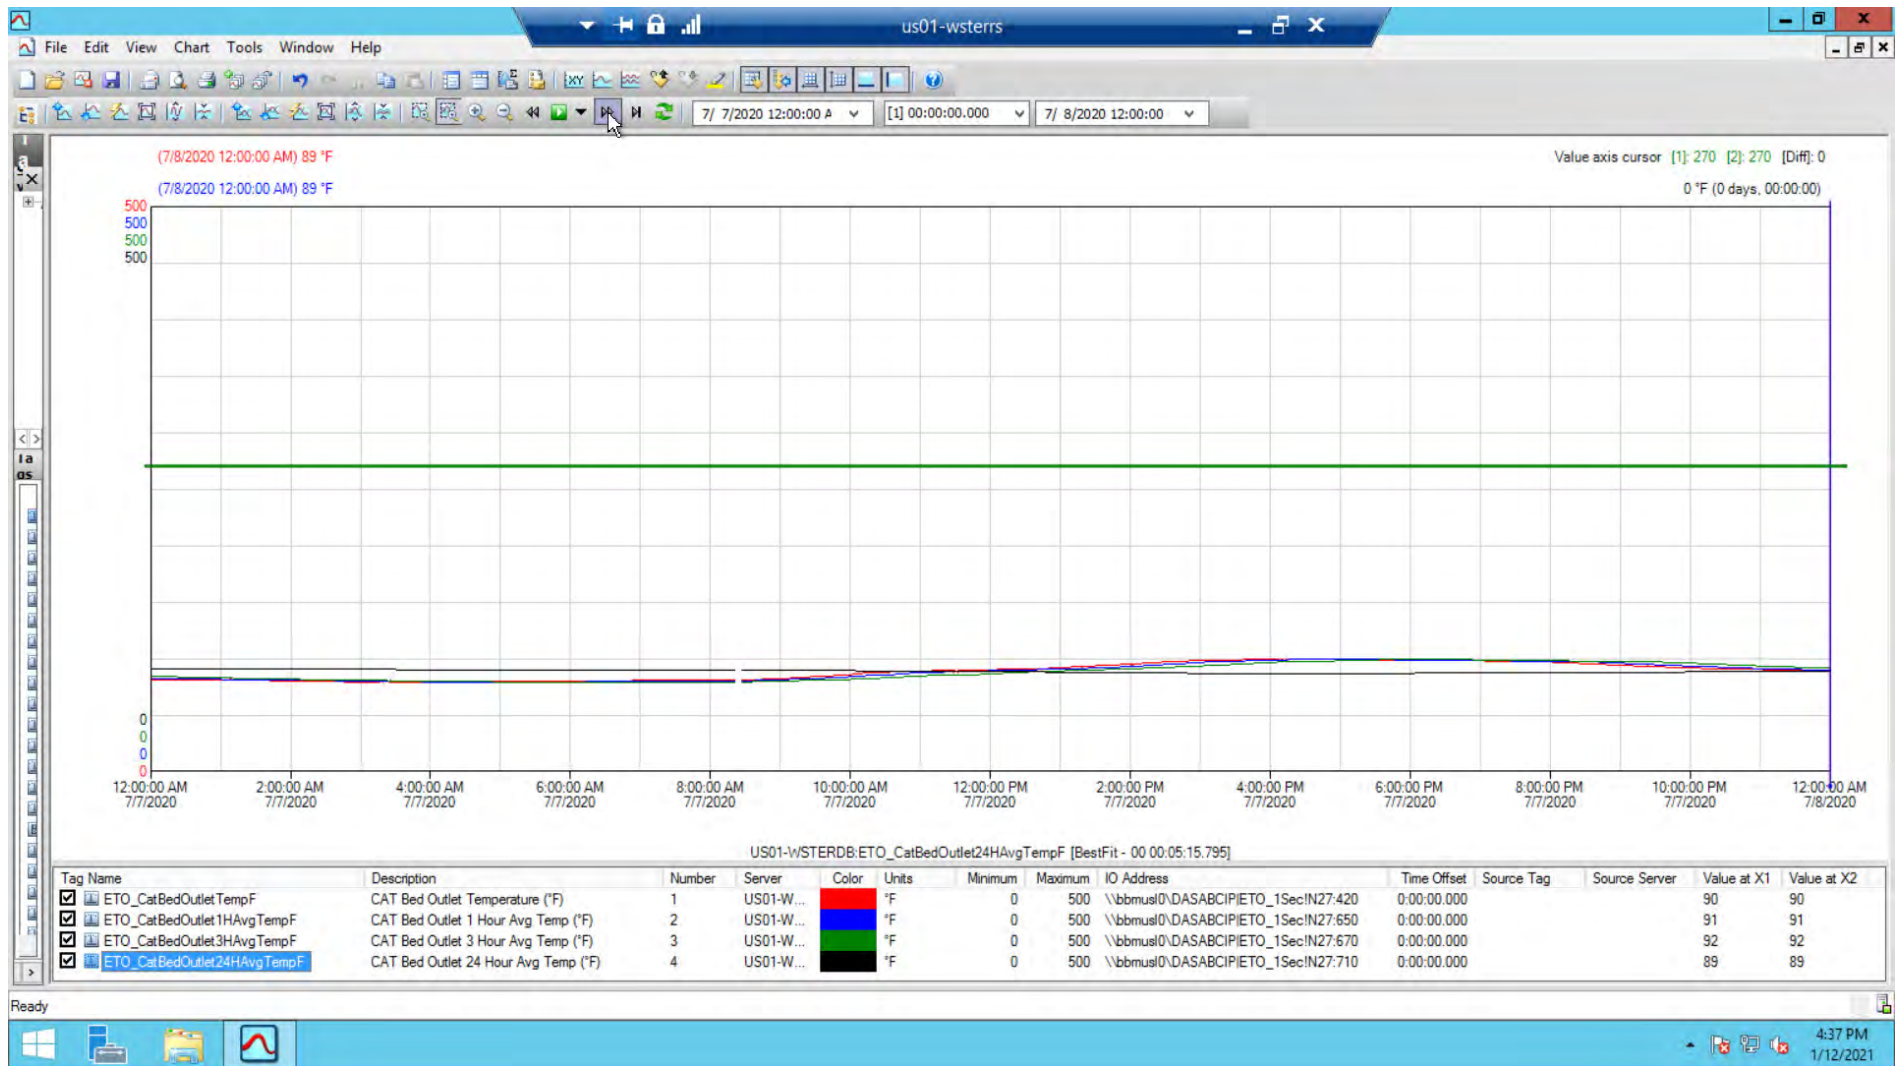

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

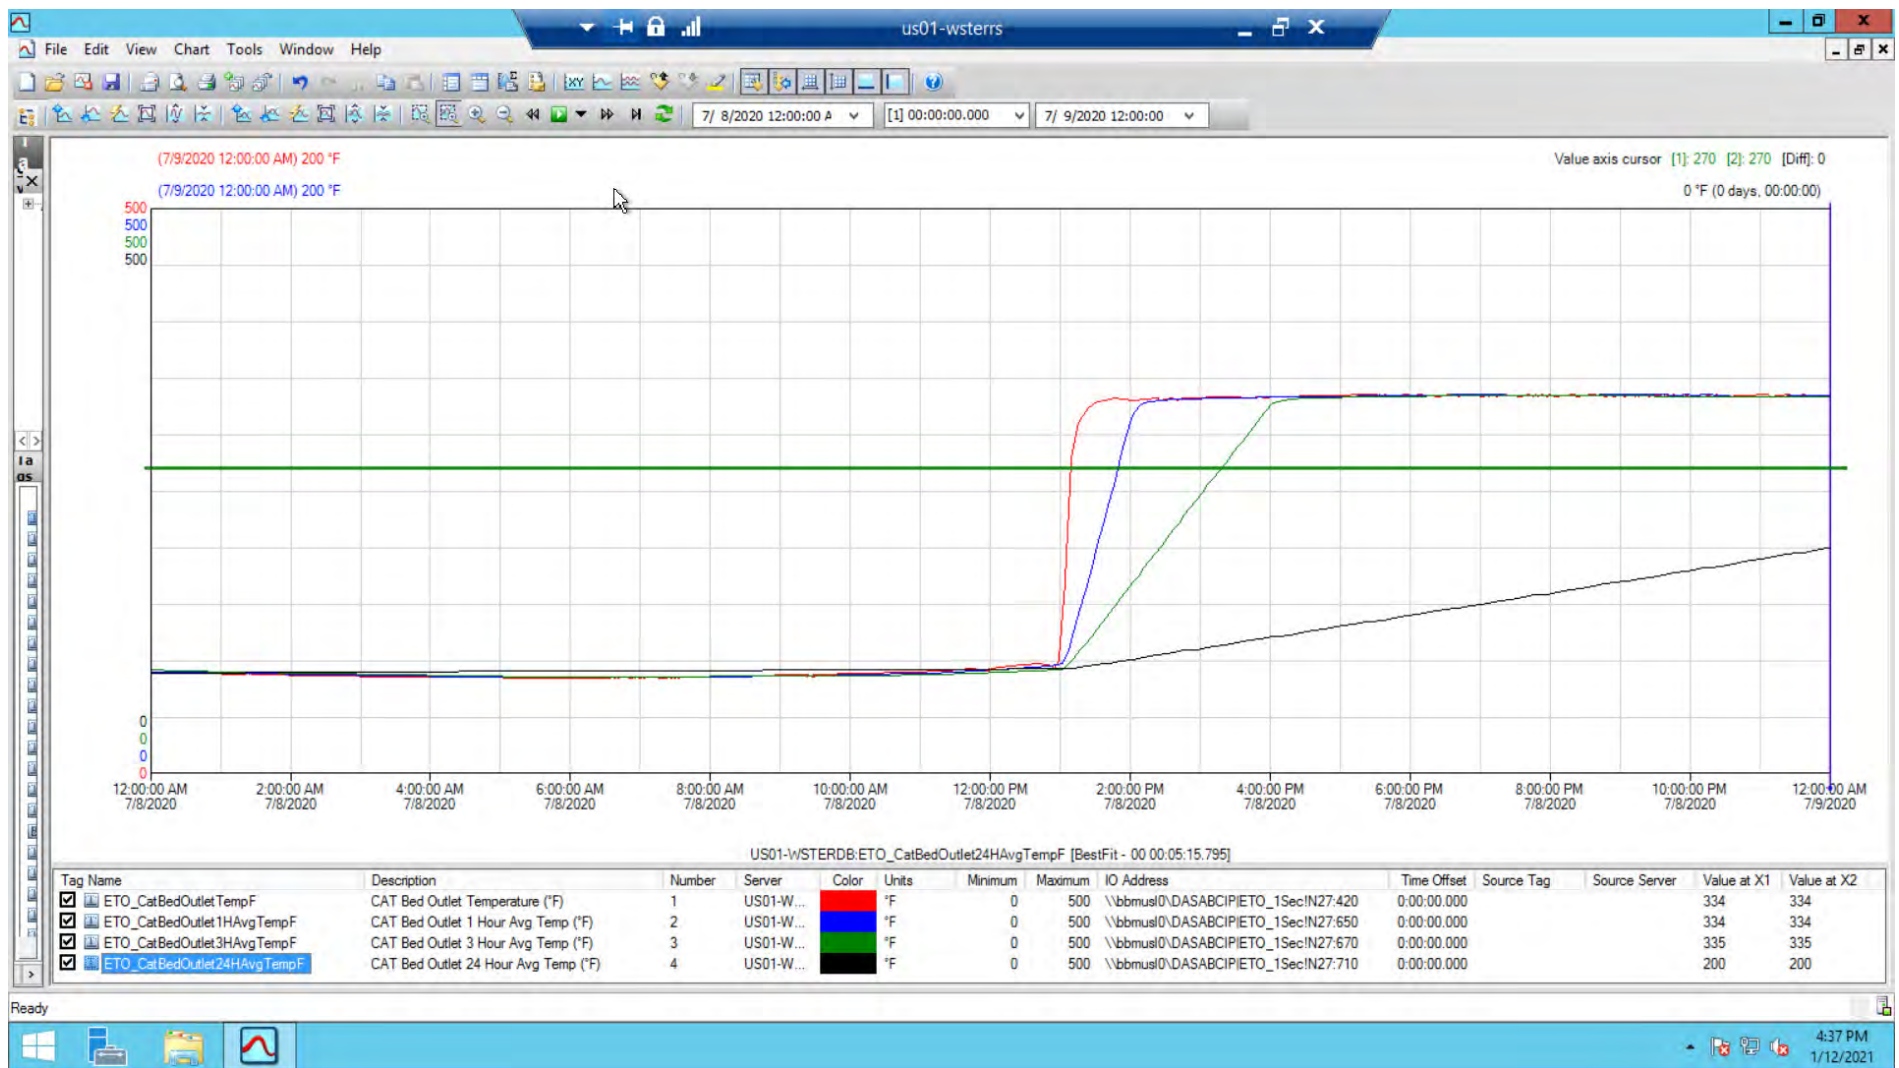


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Jul 2020

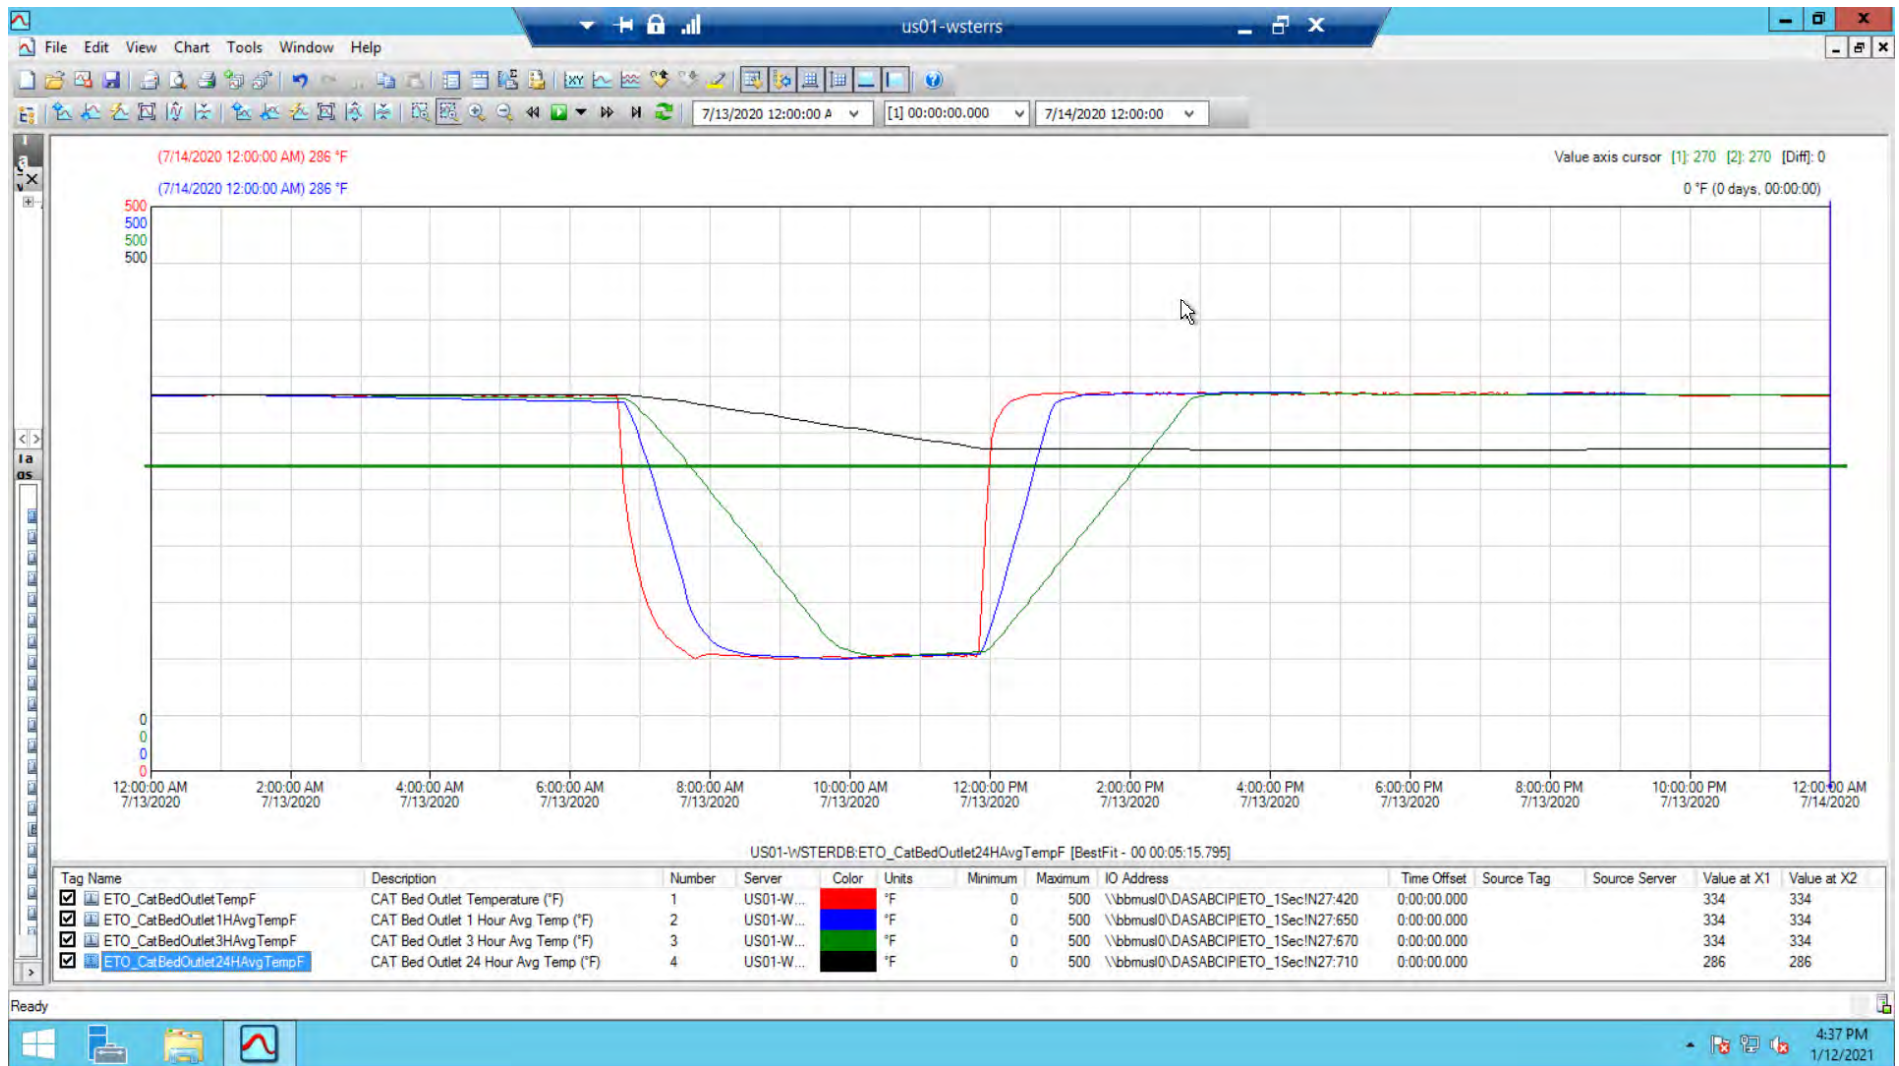



# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

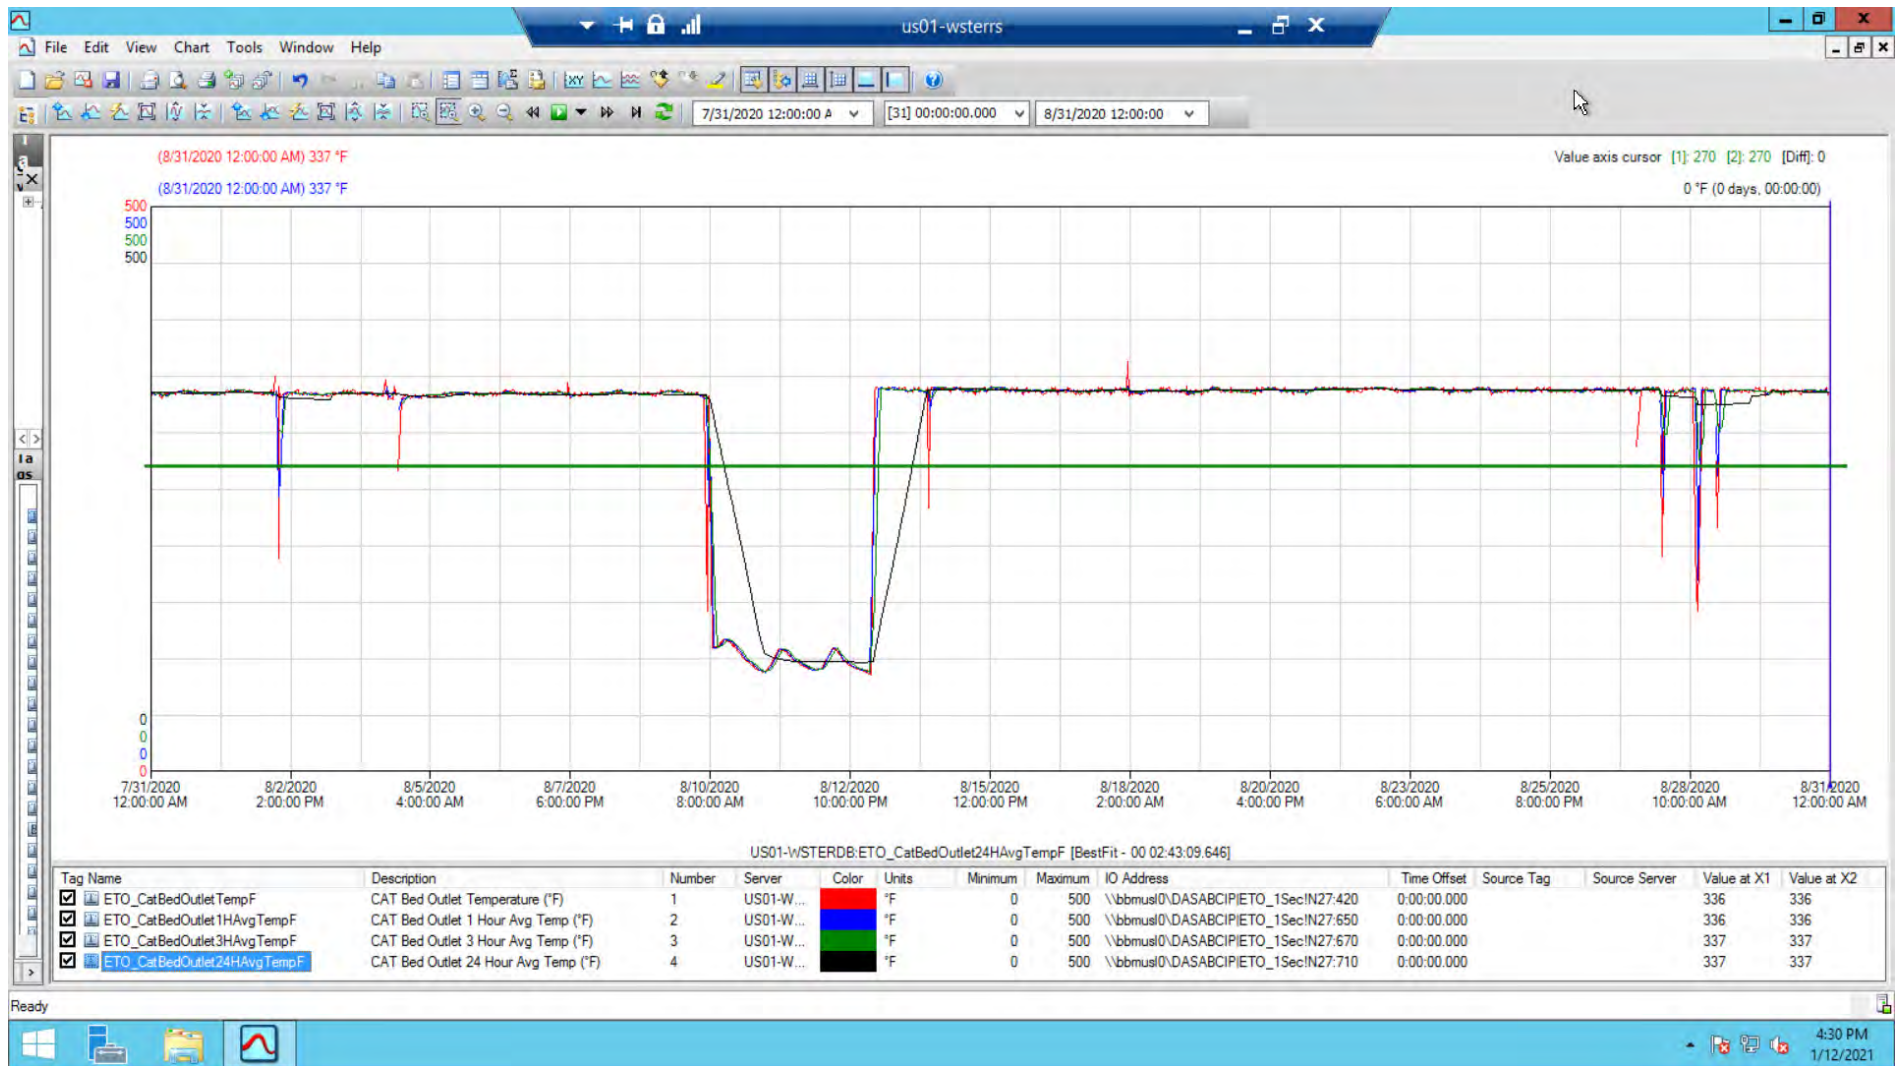





# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020



# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

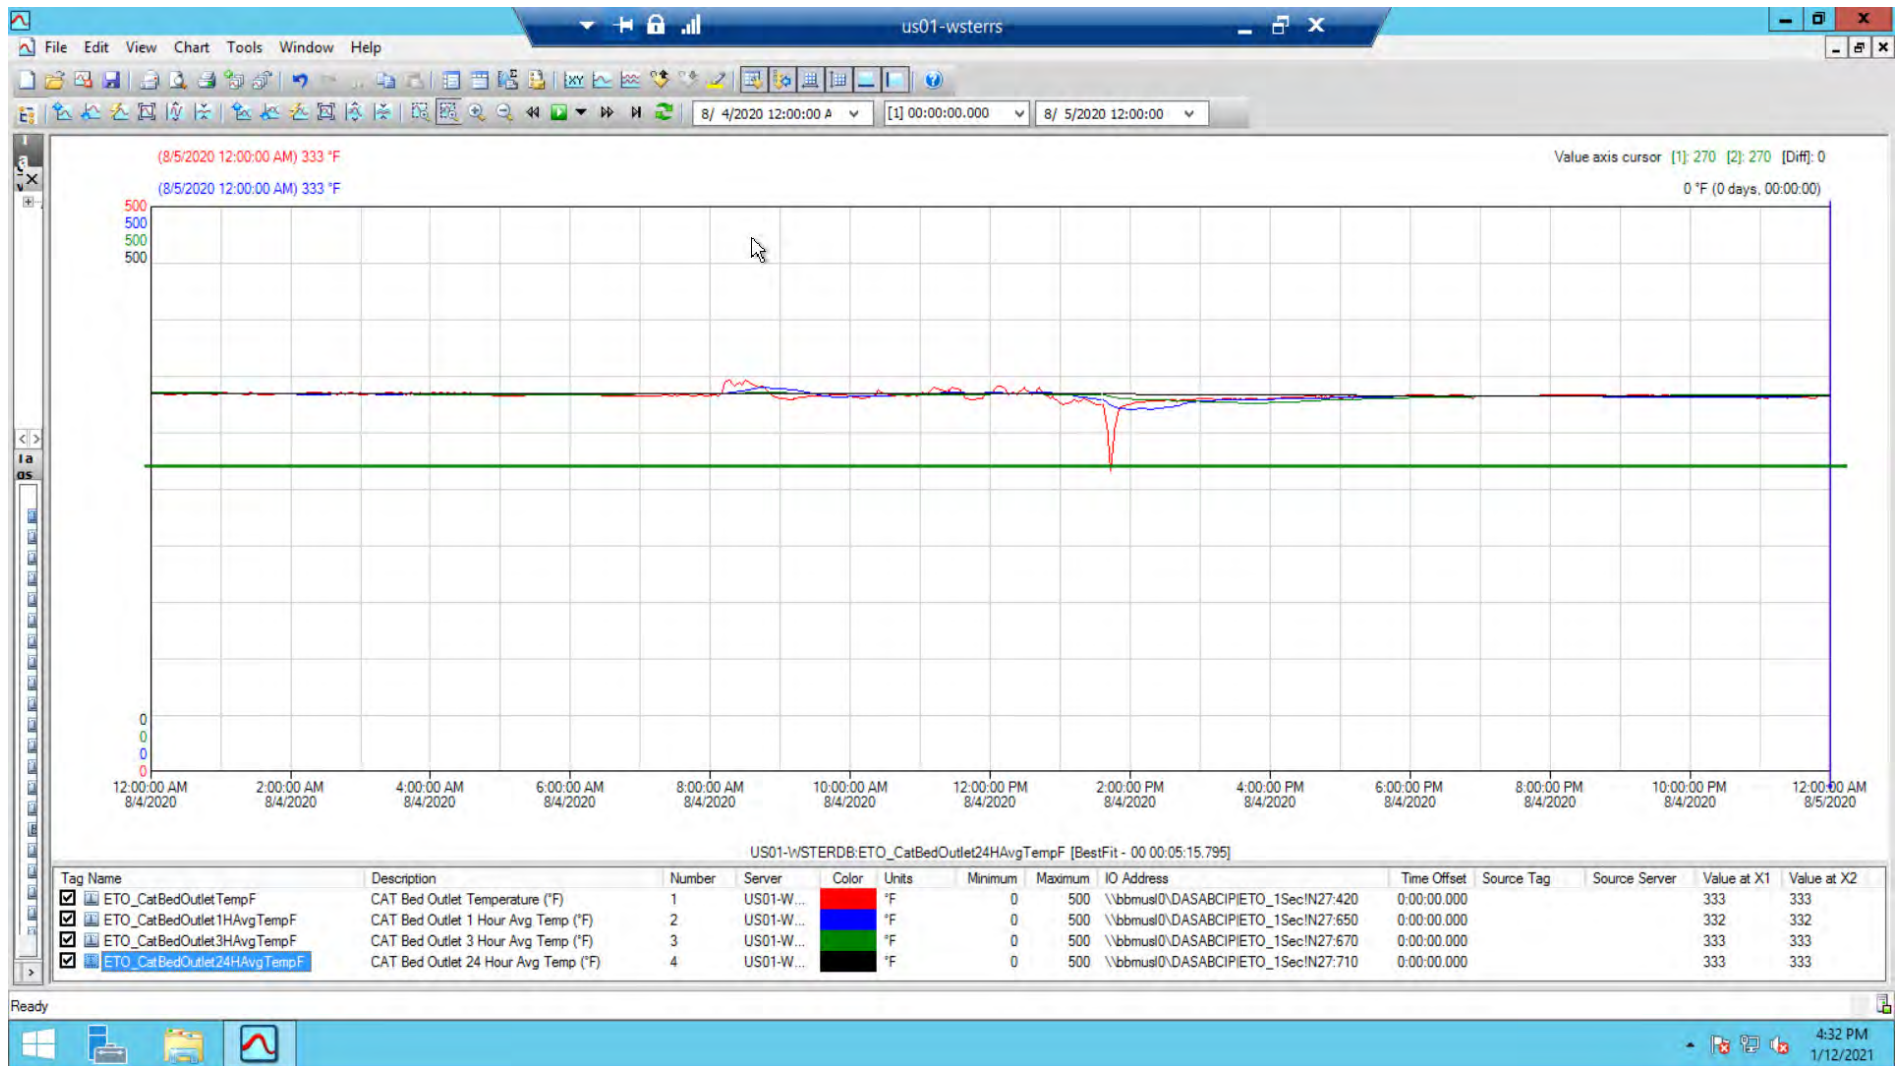


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

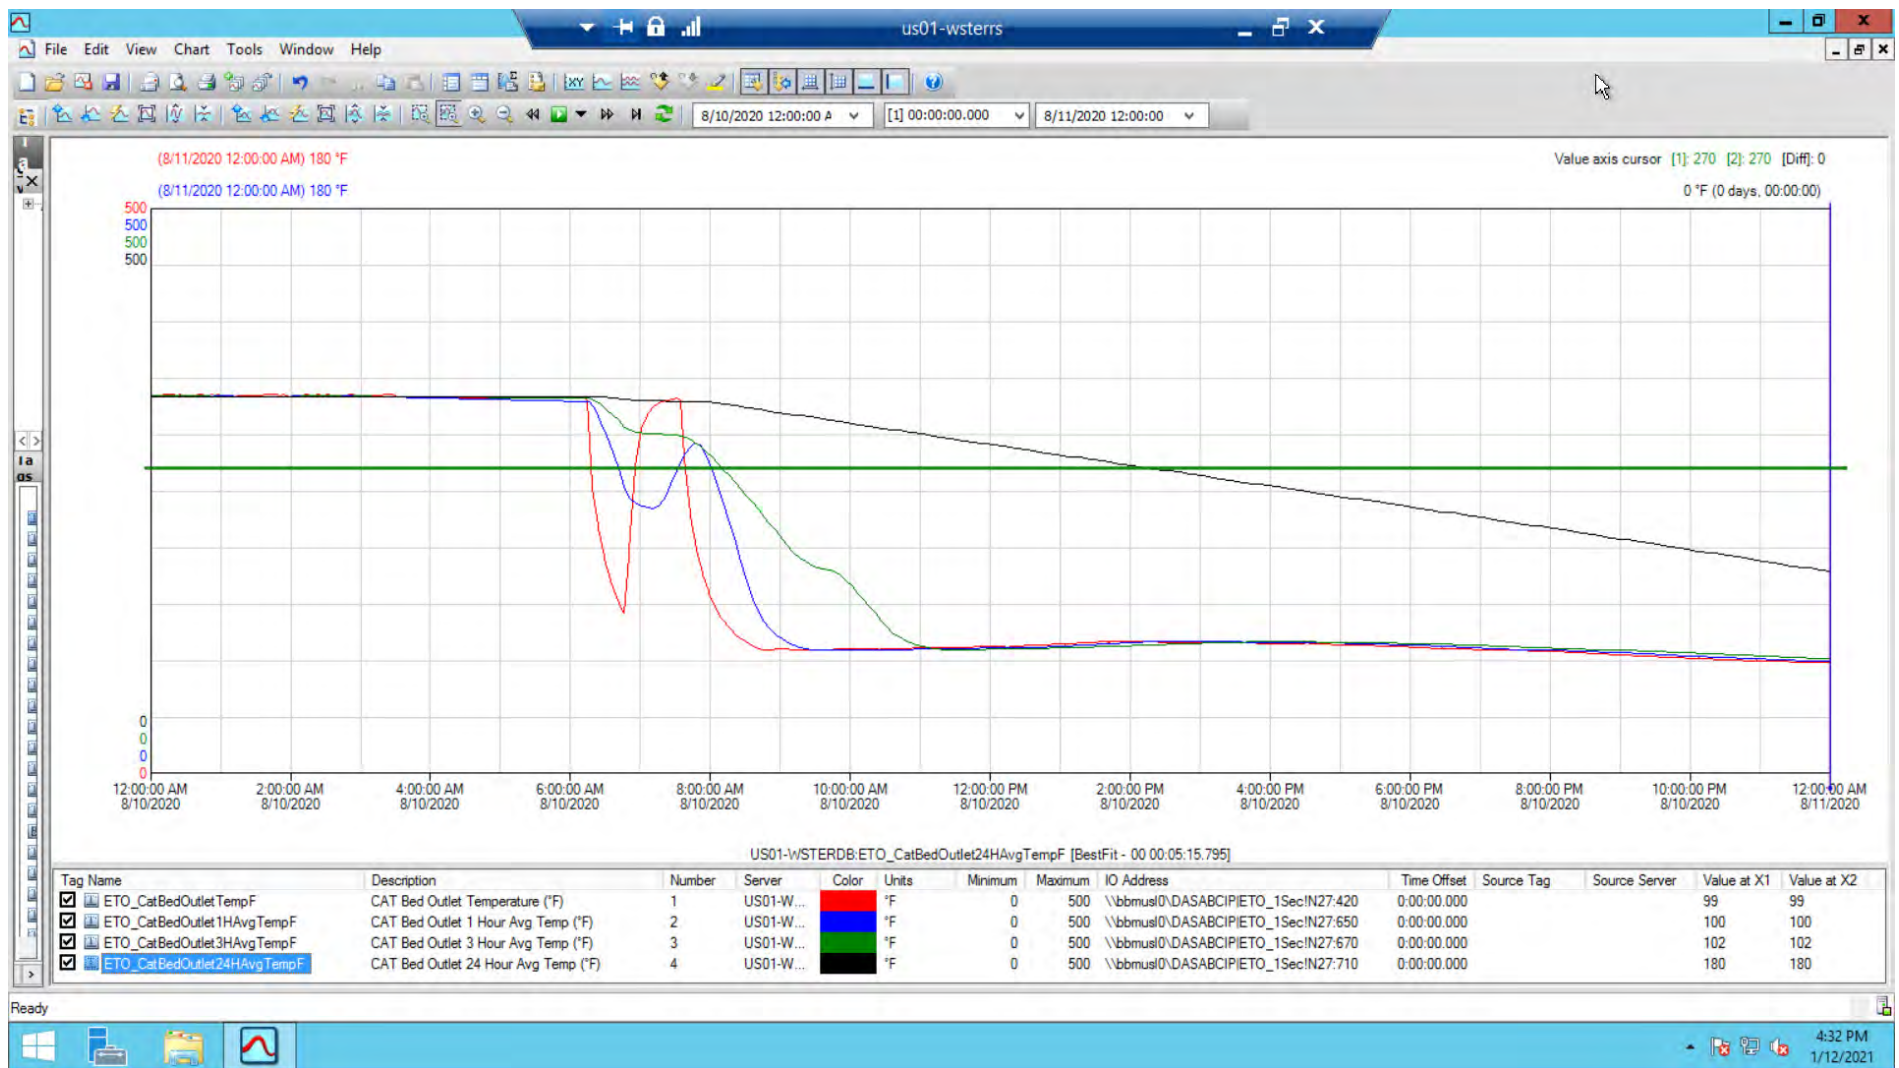




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

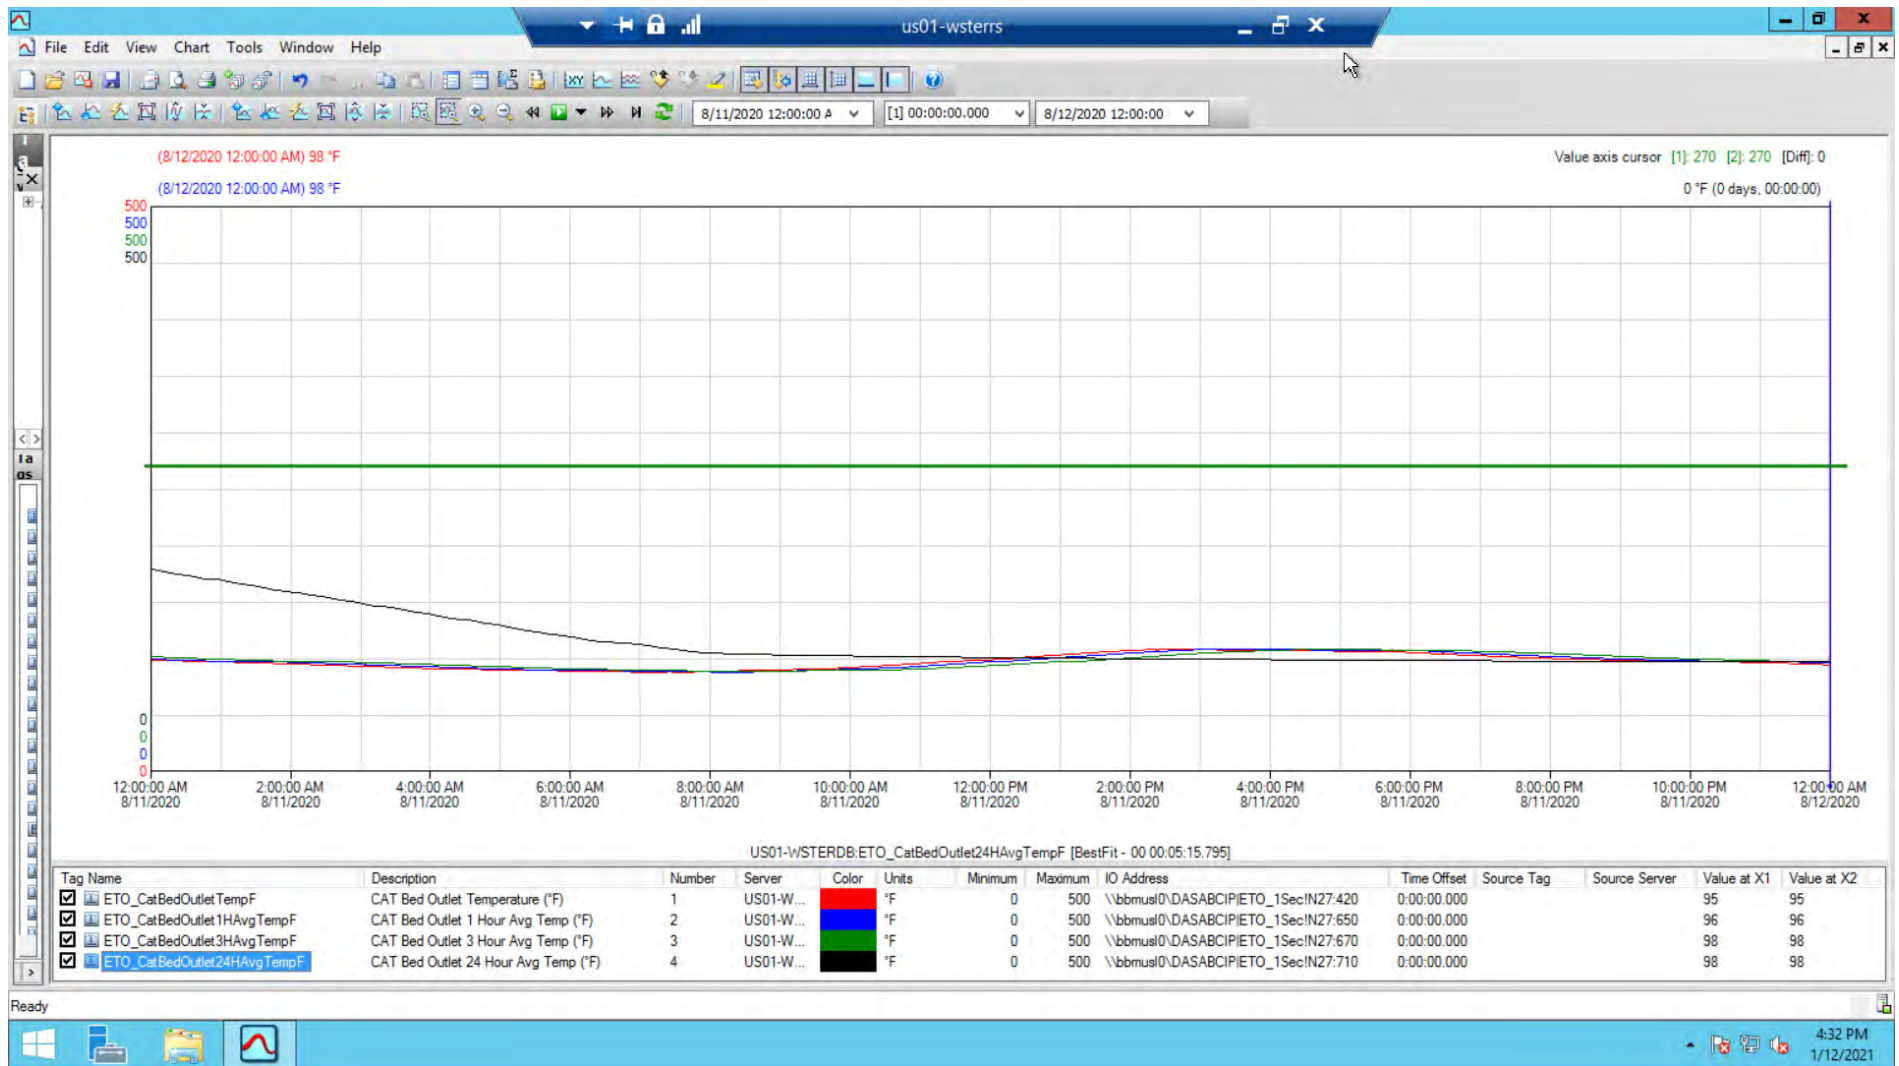




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

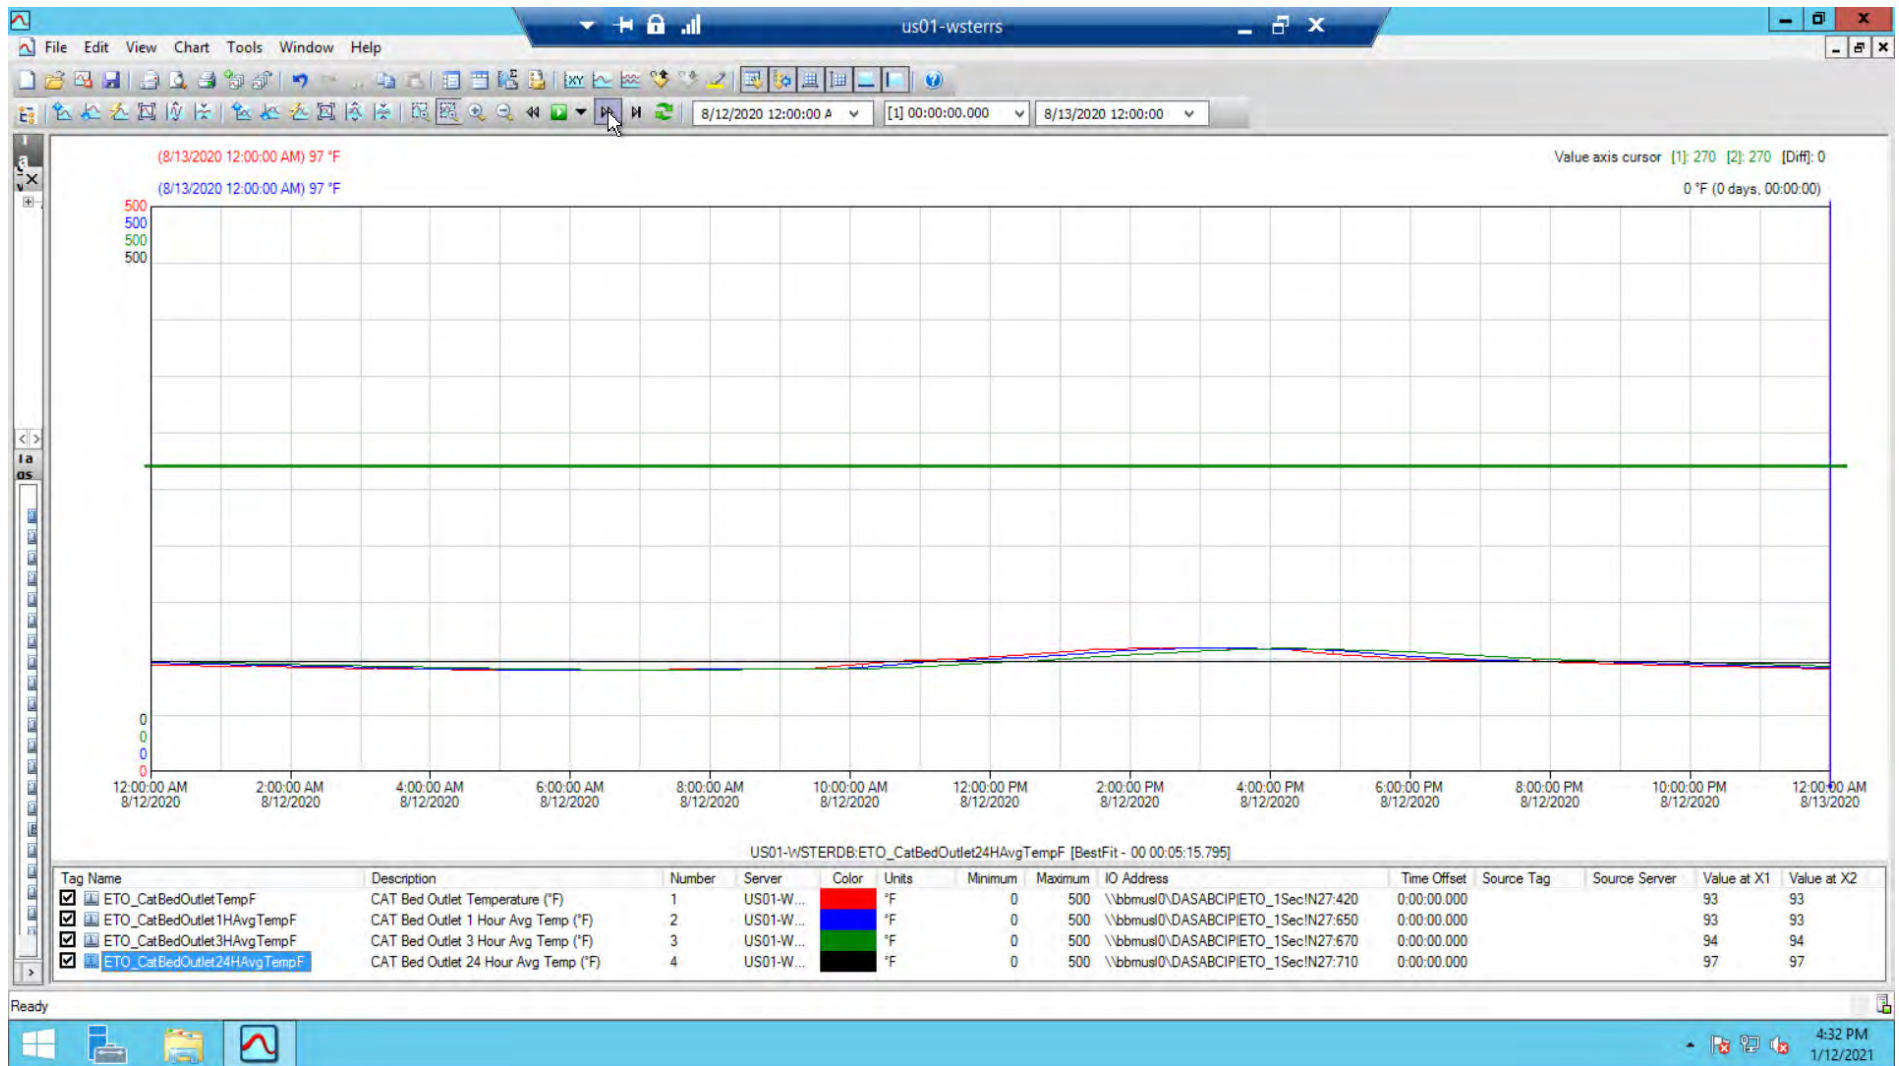

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

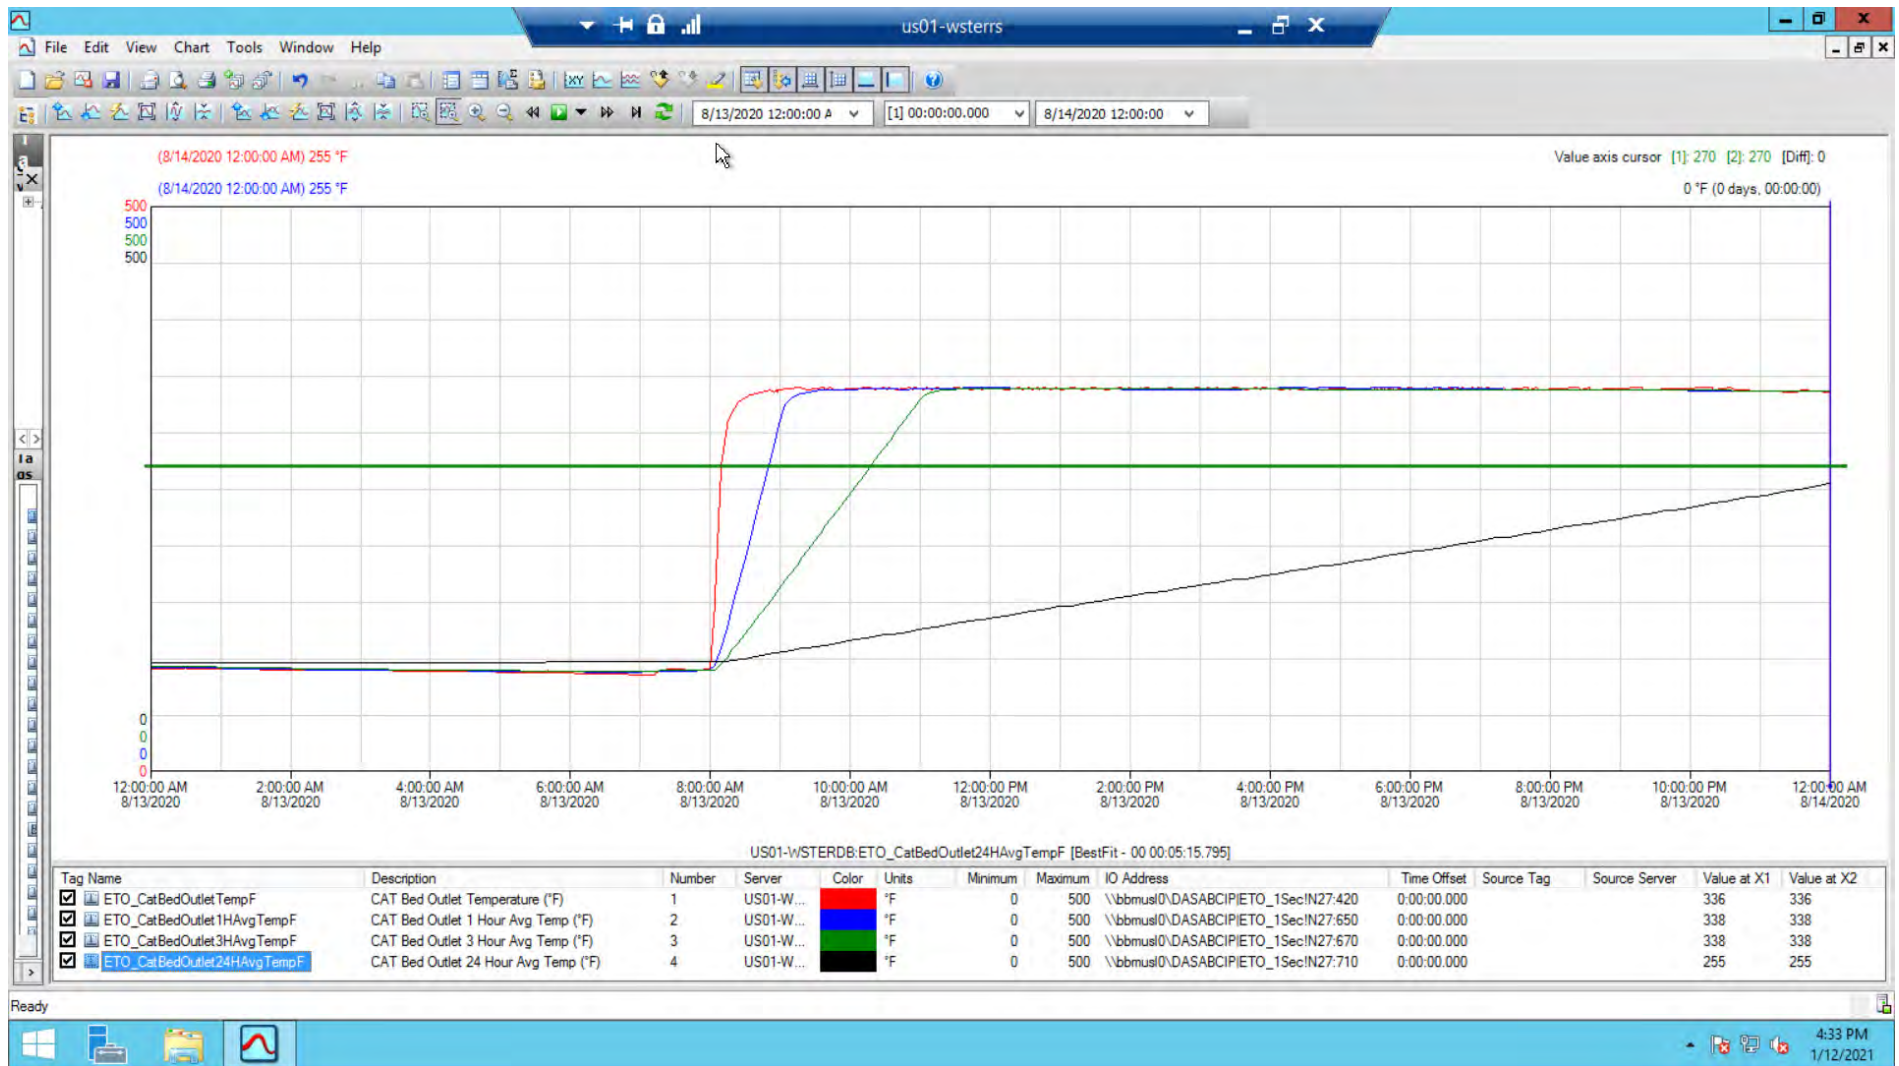


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020






# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

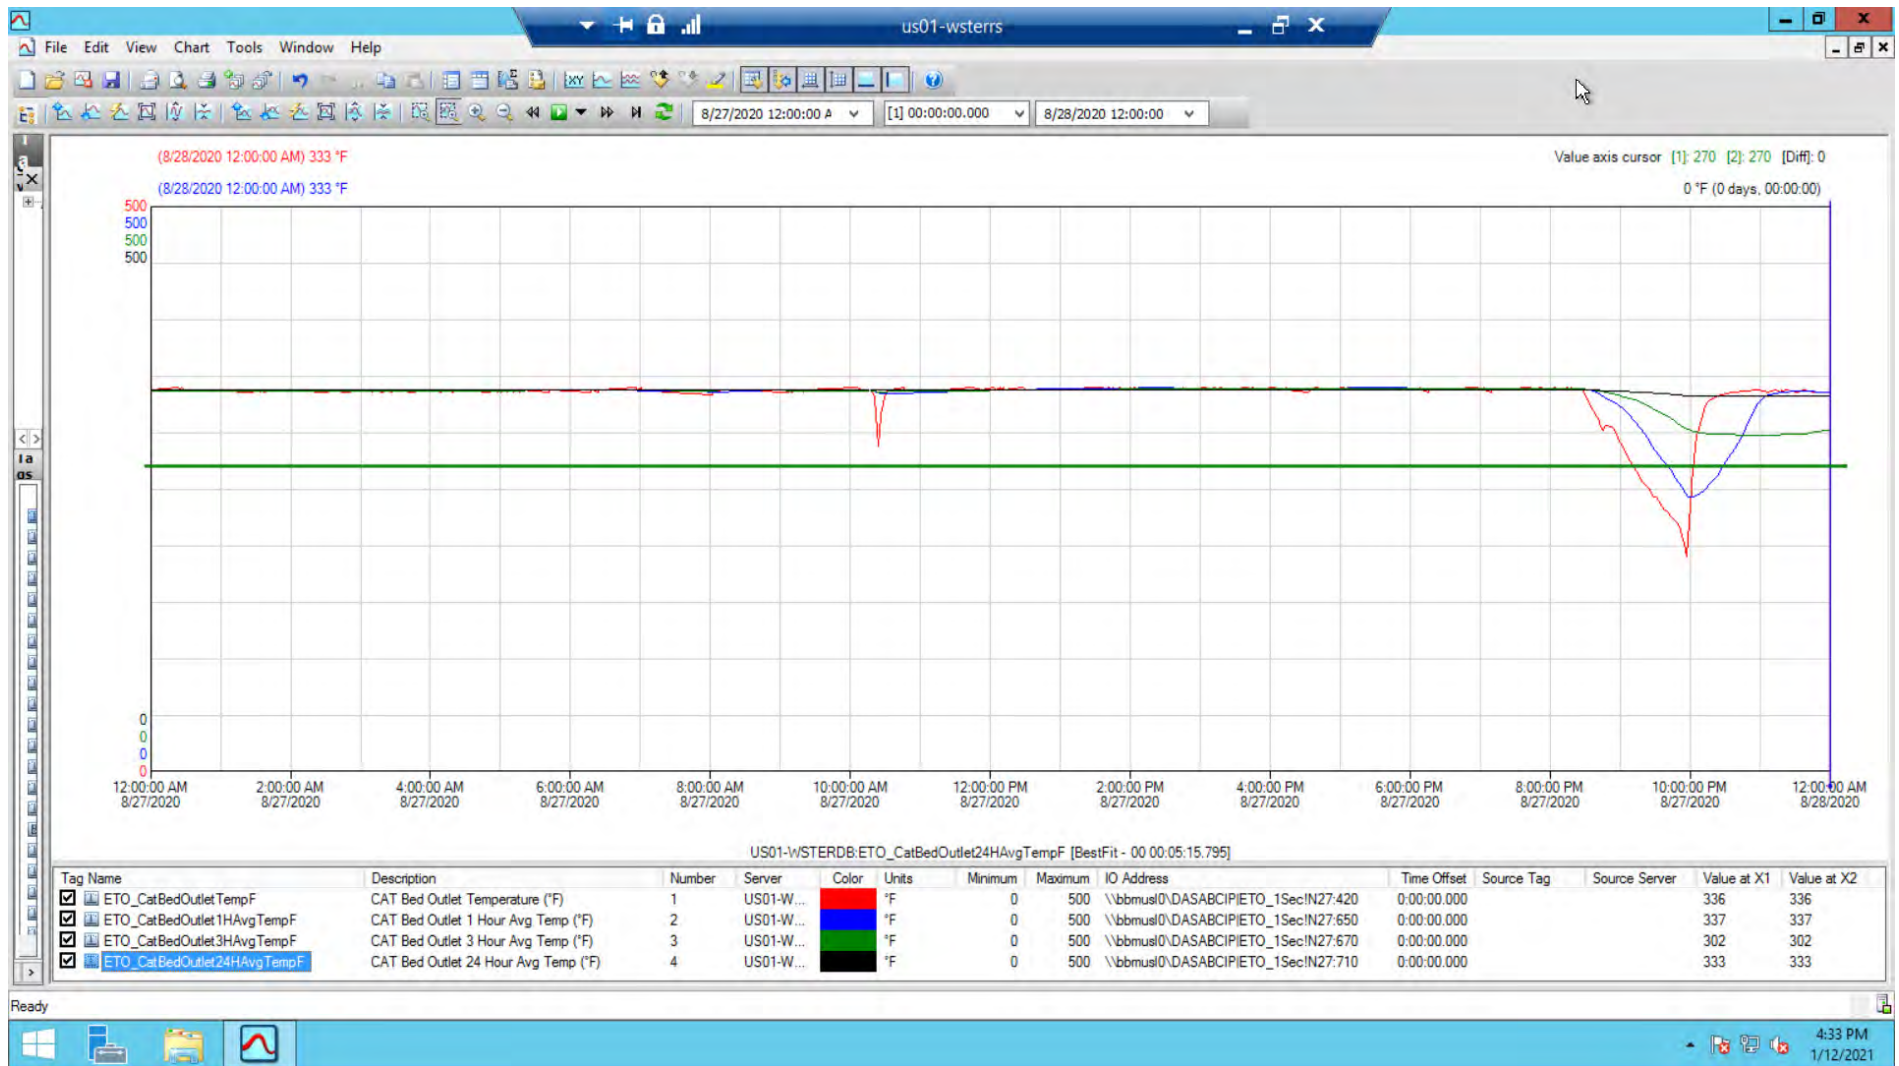





# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Aug 2020

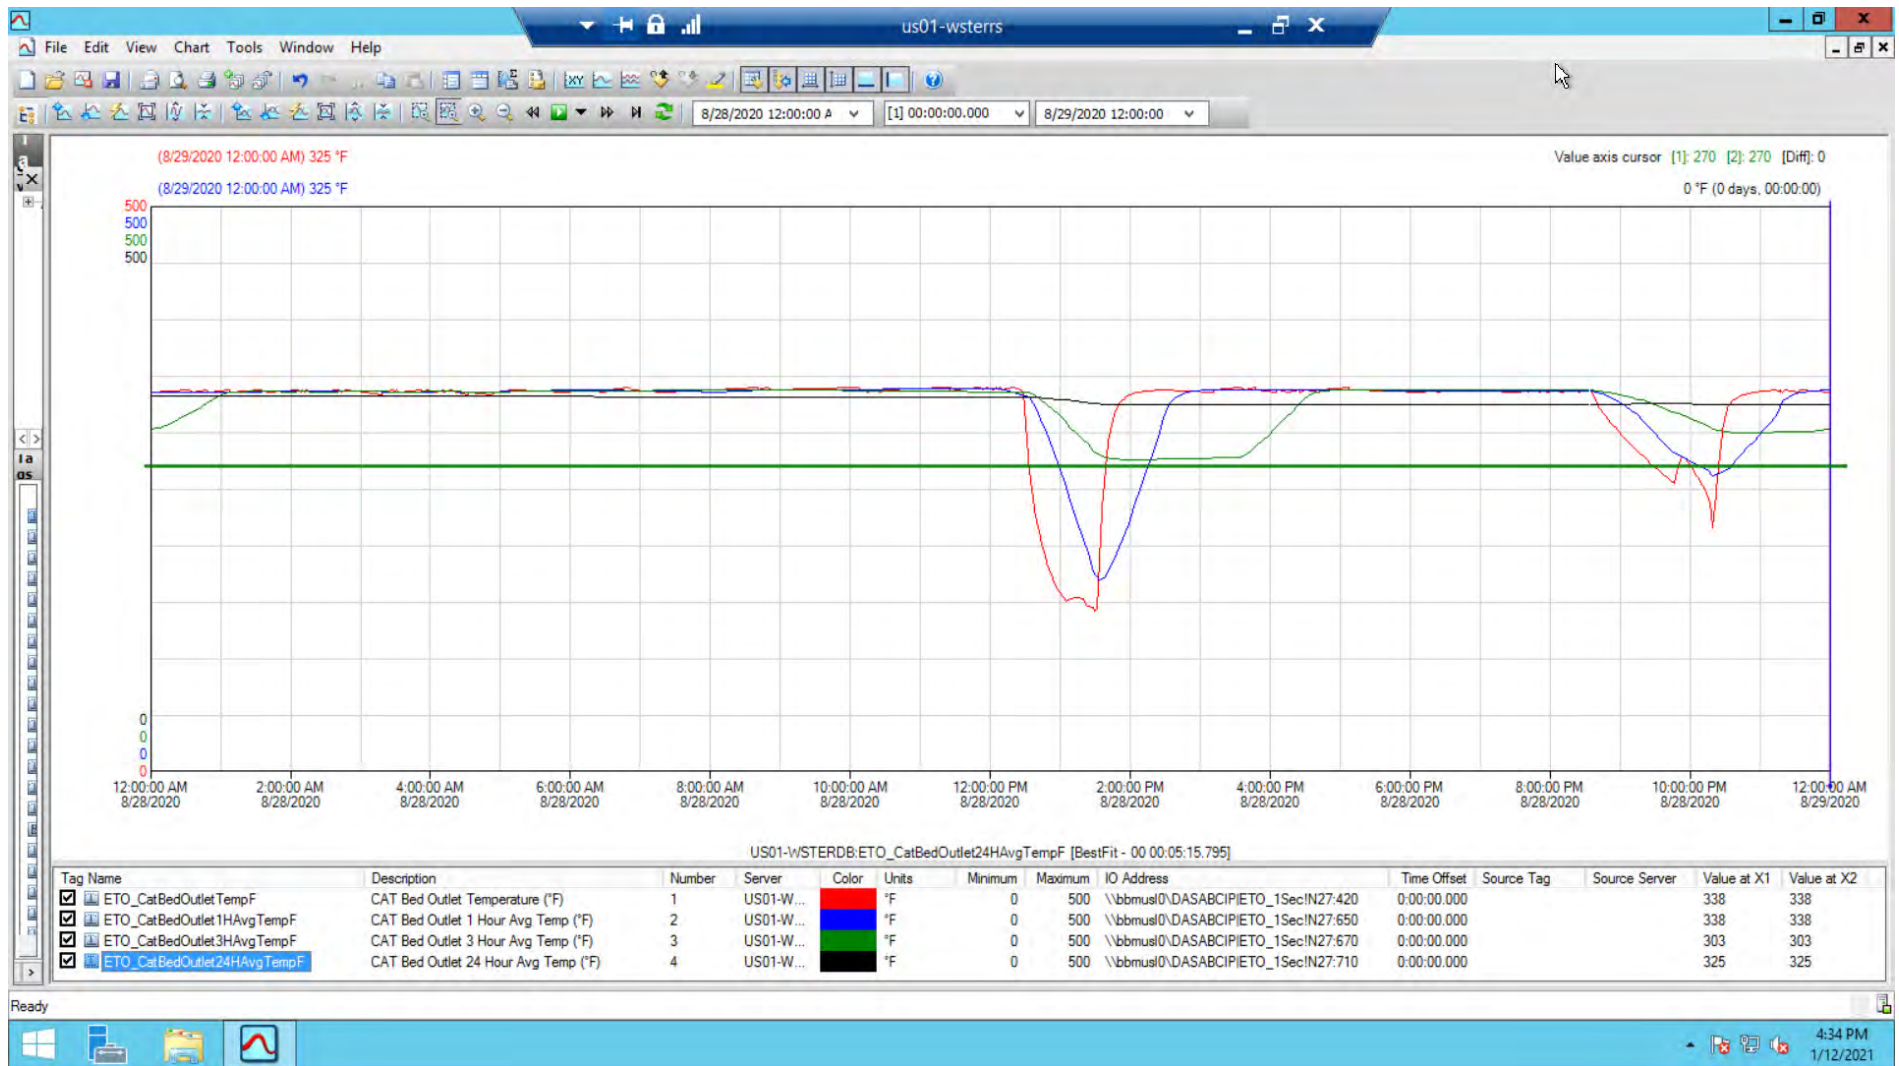

# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Sep 2020

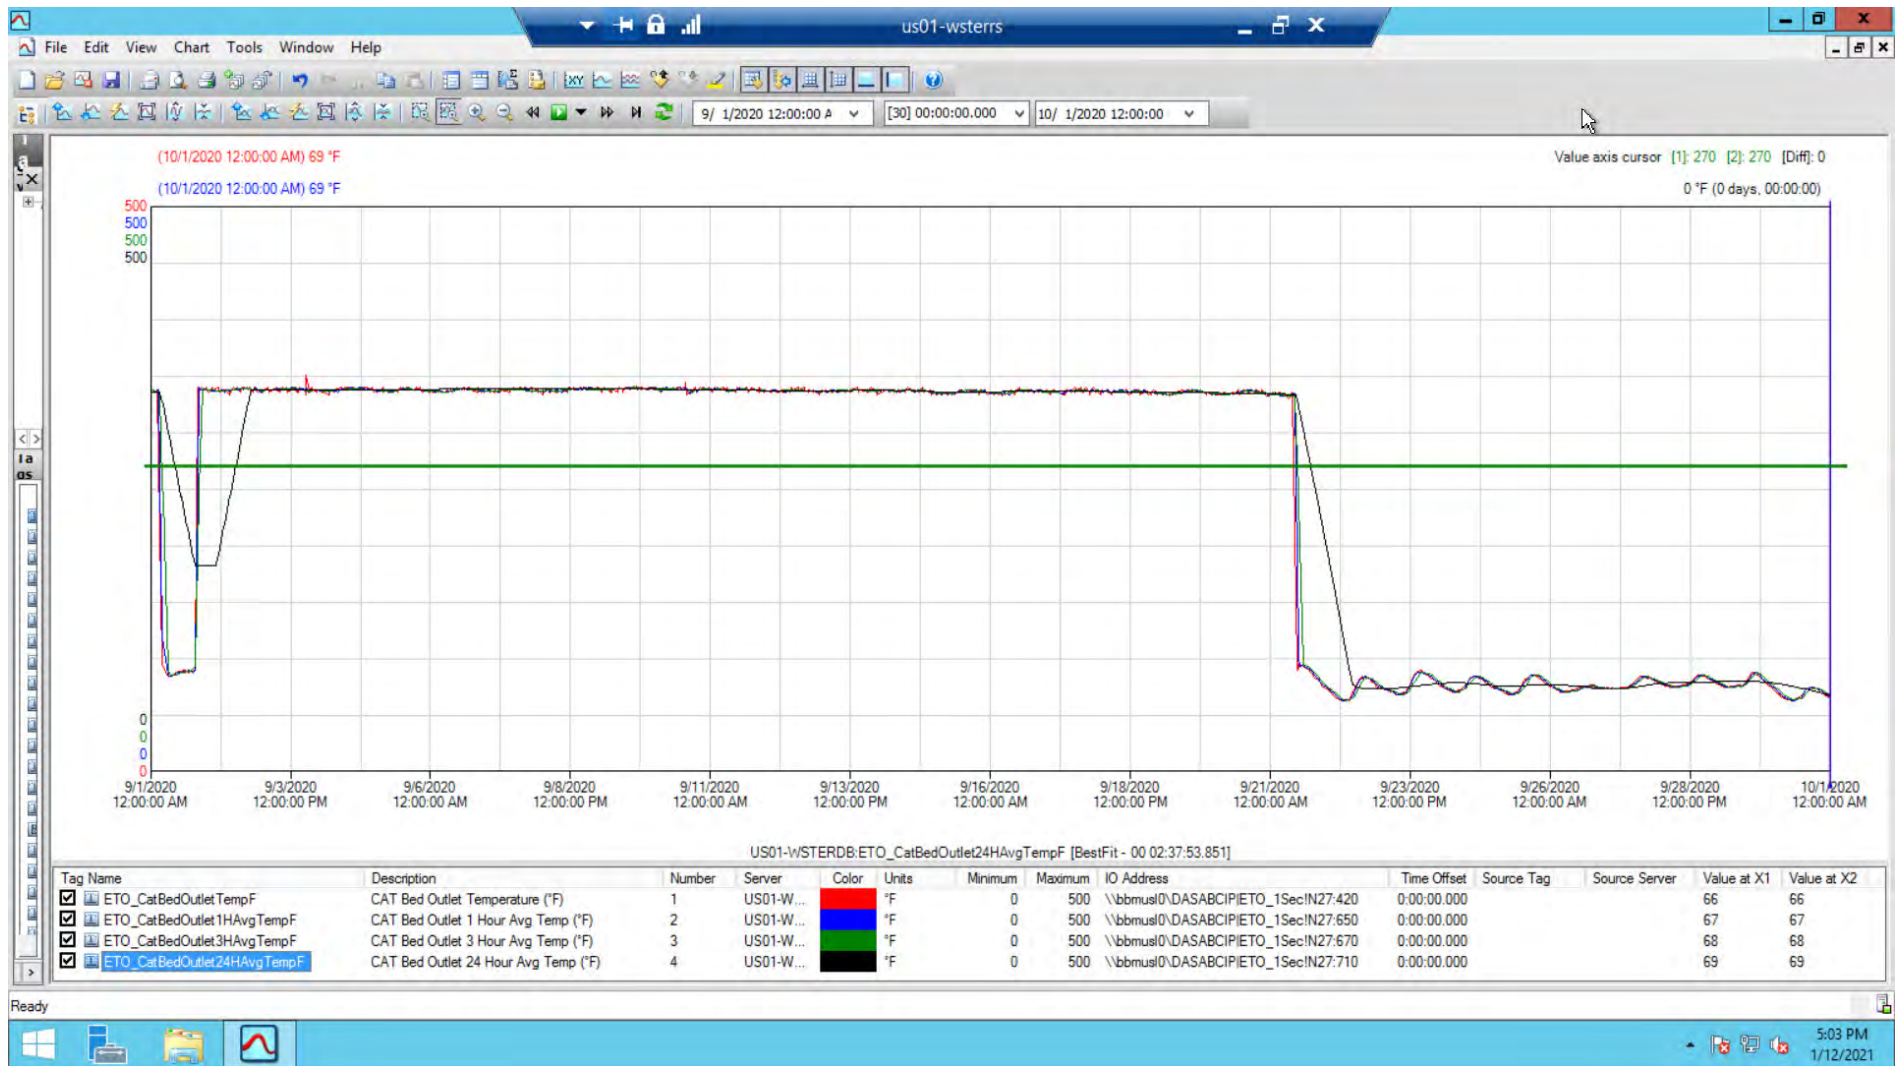


# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Sep 2020

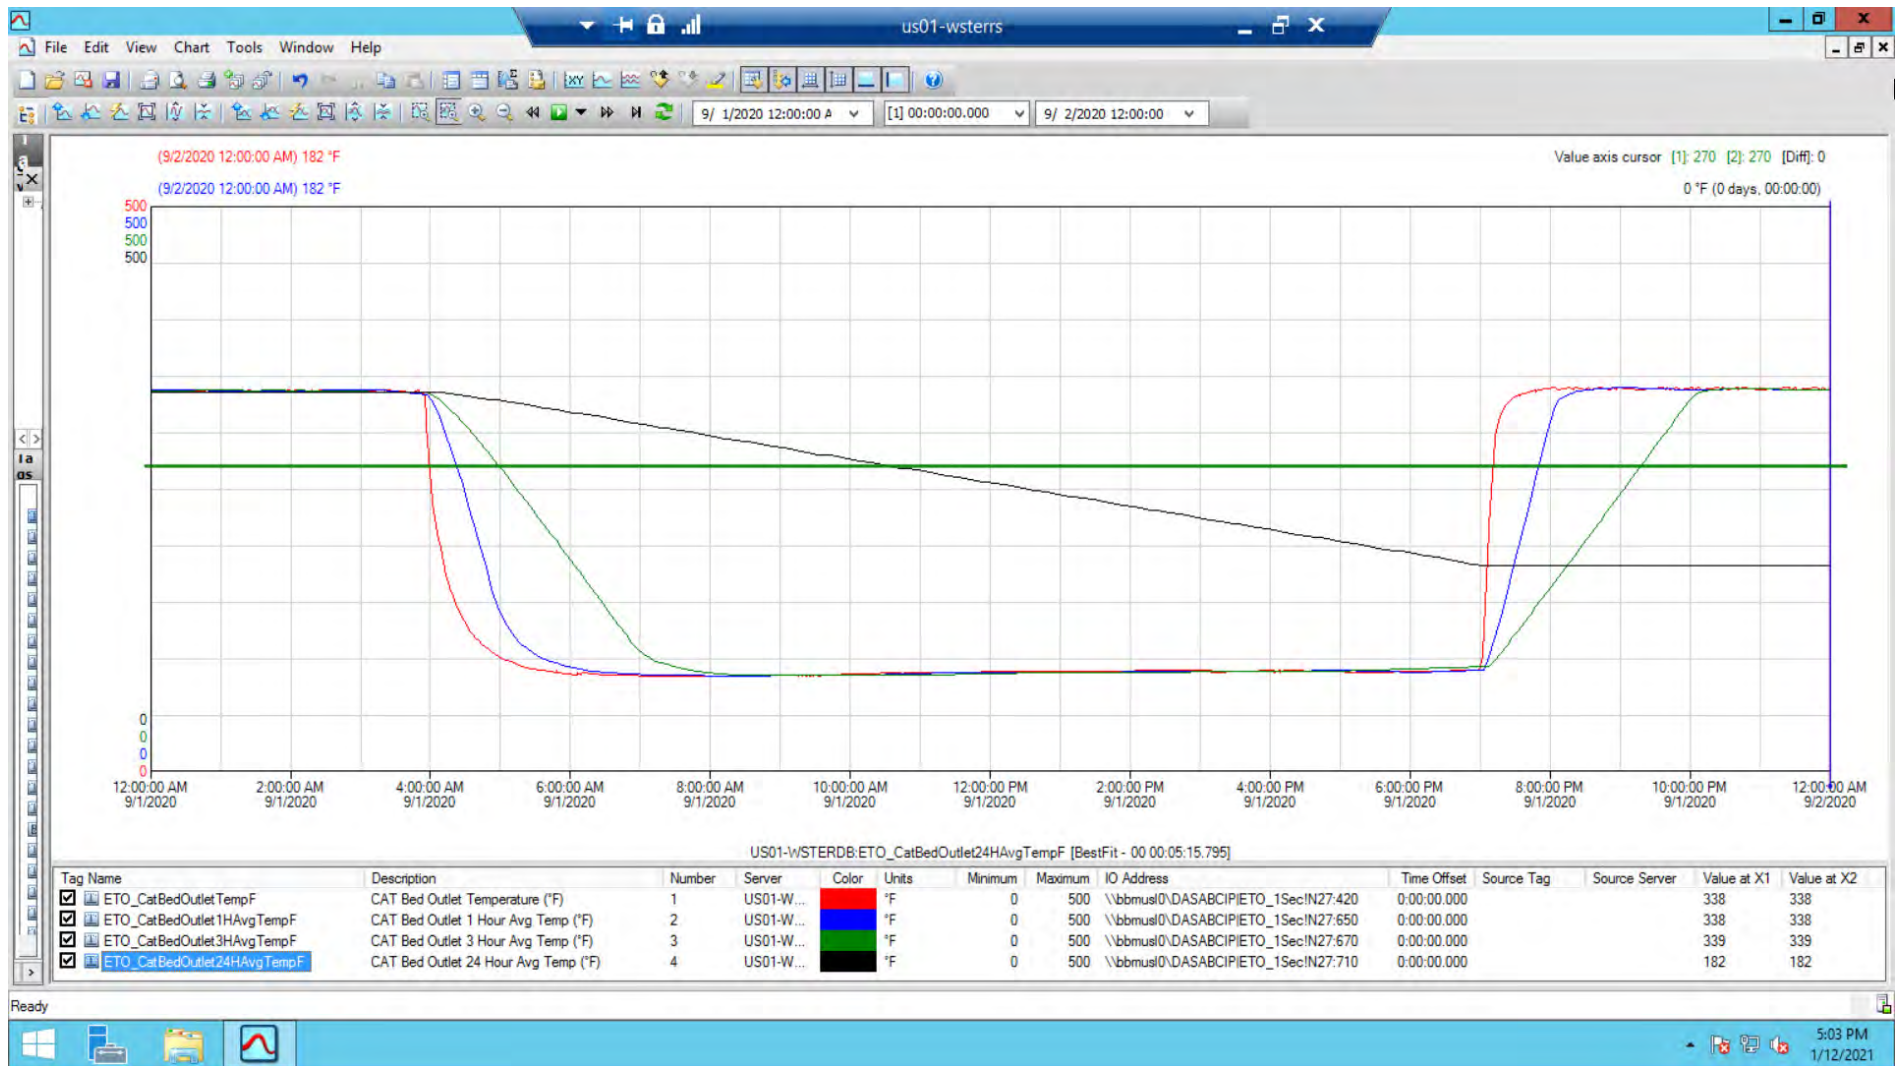




# B Braun Medical Allentown Facility (EO Bed Outlet Temperature (degrees F)) – Sep 2020

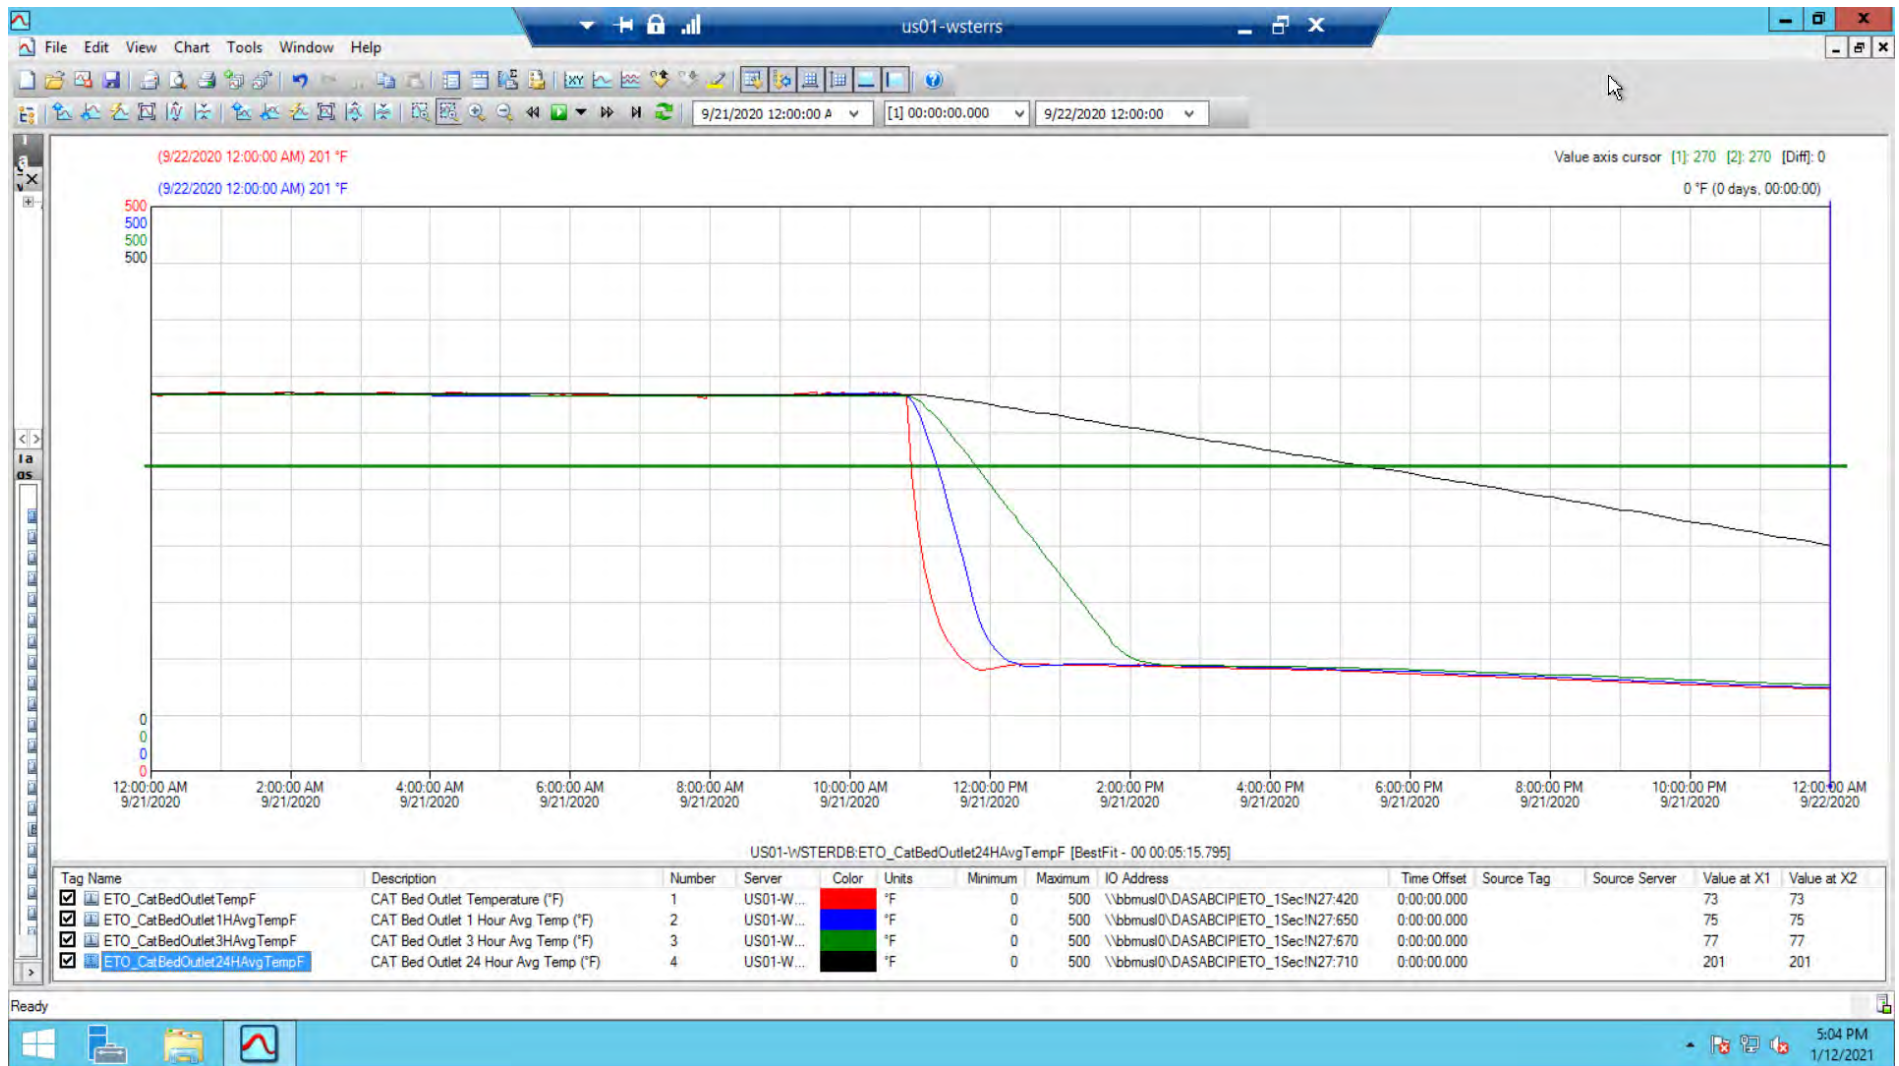




# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Oct 2020

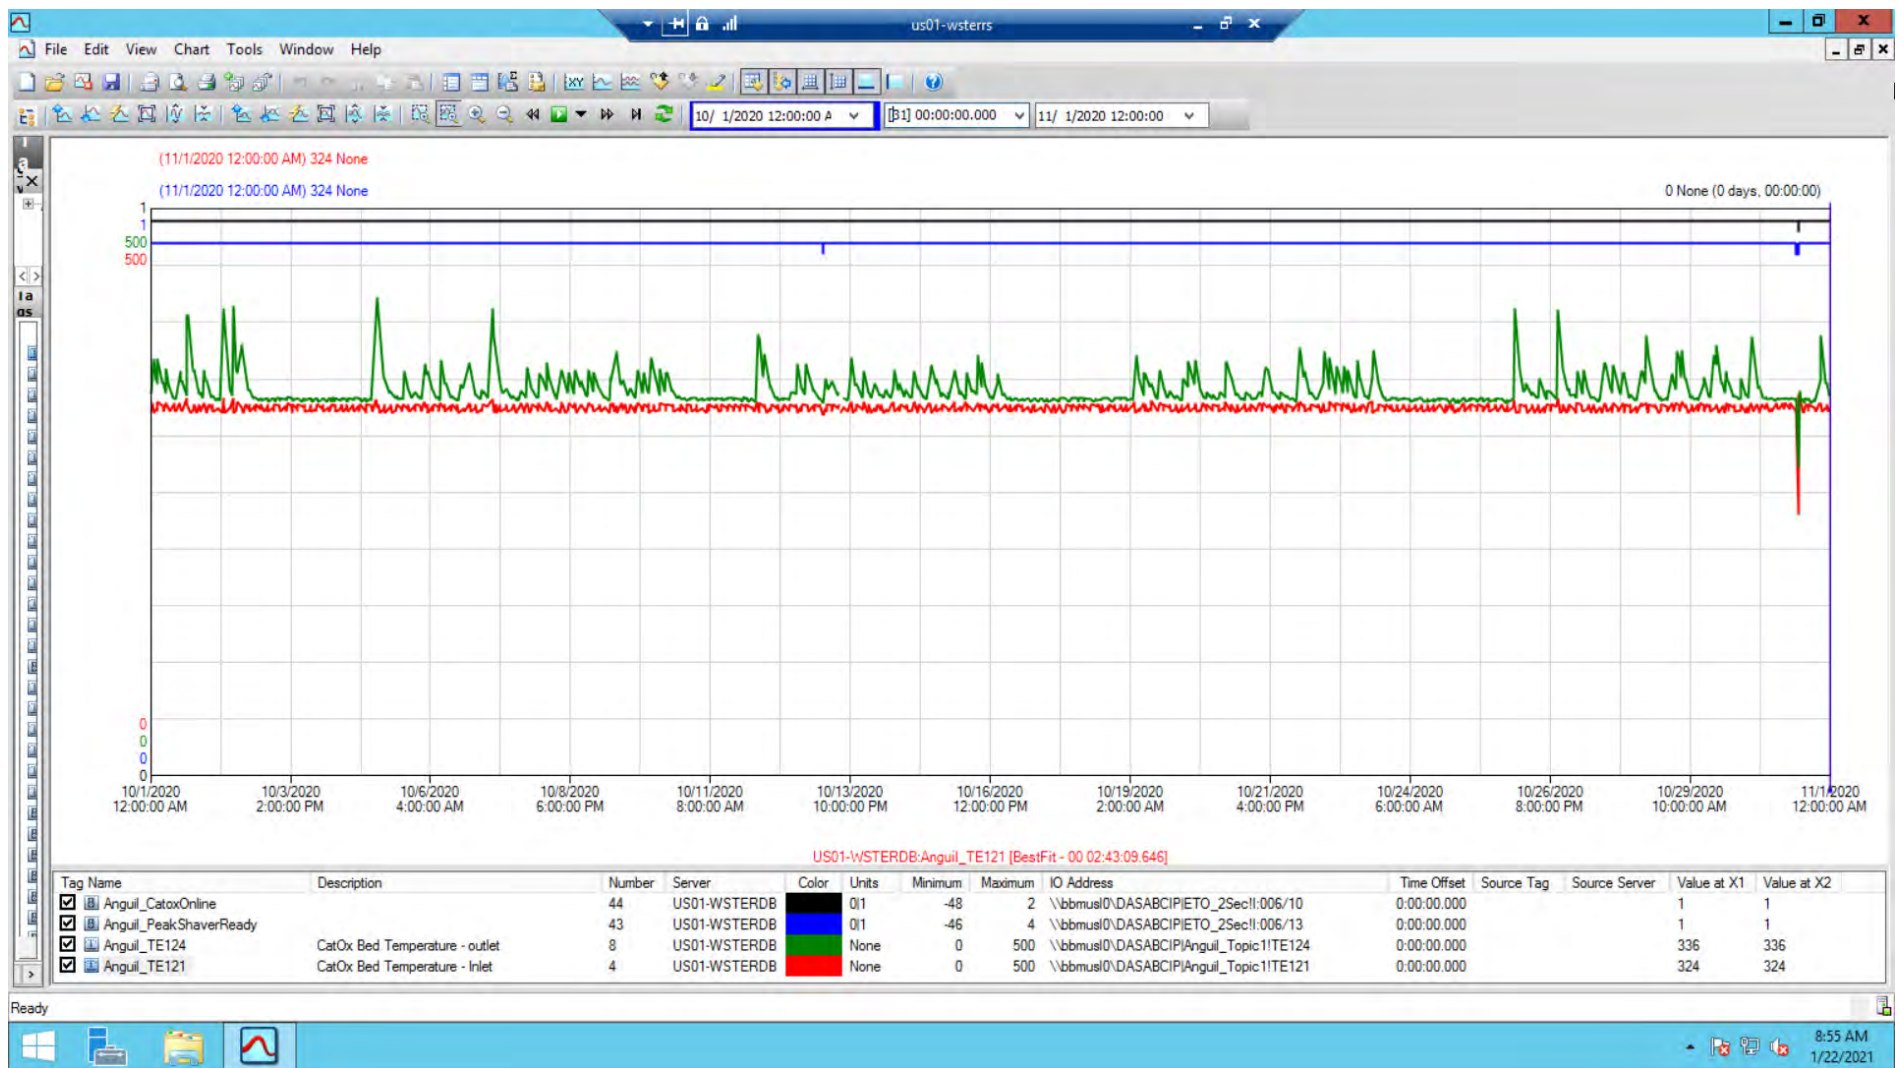

# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Oct 2020



# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Nov 2020

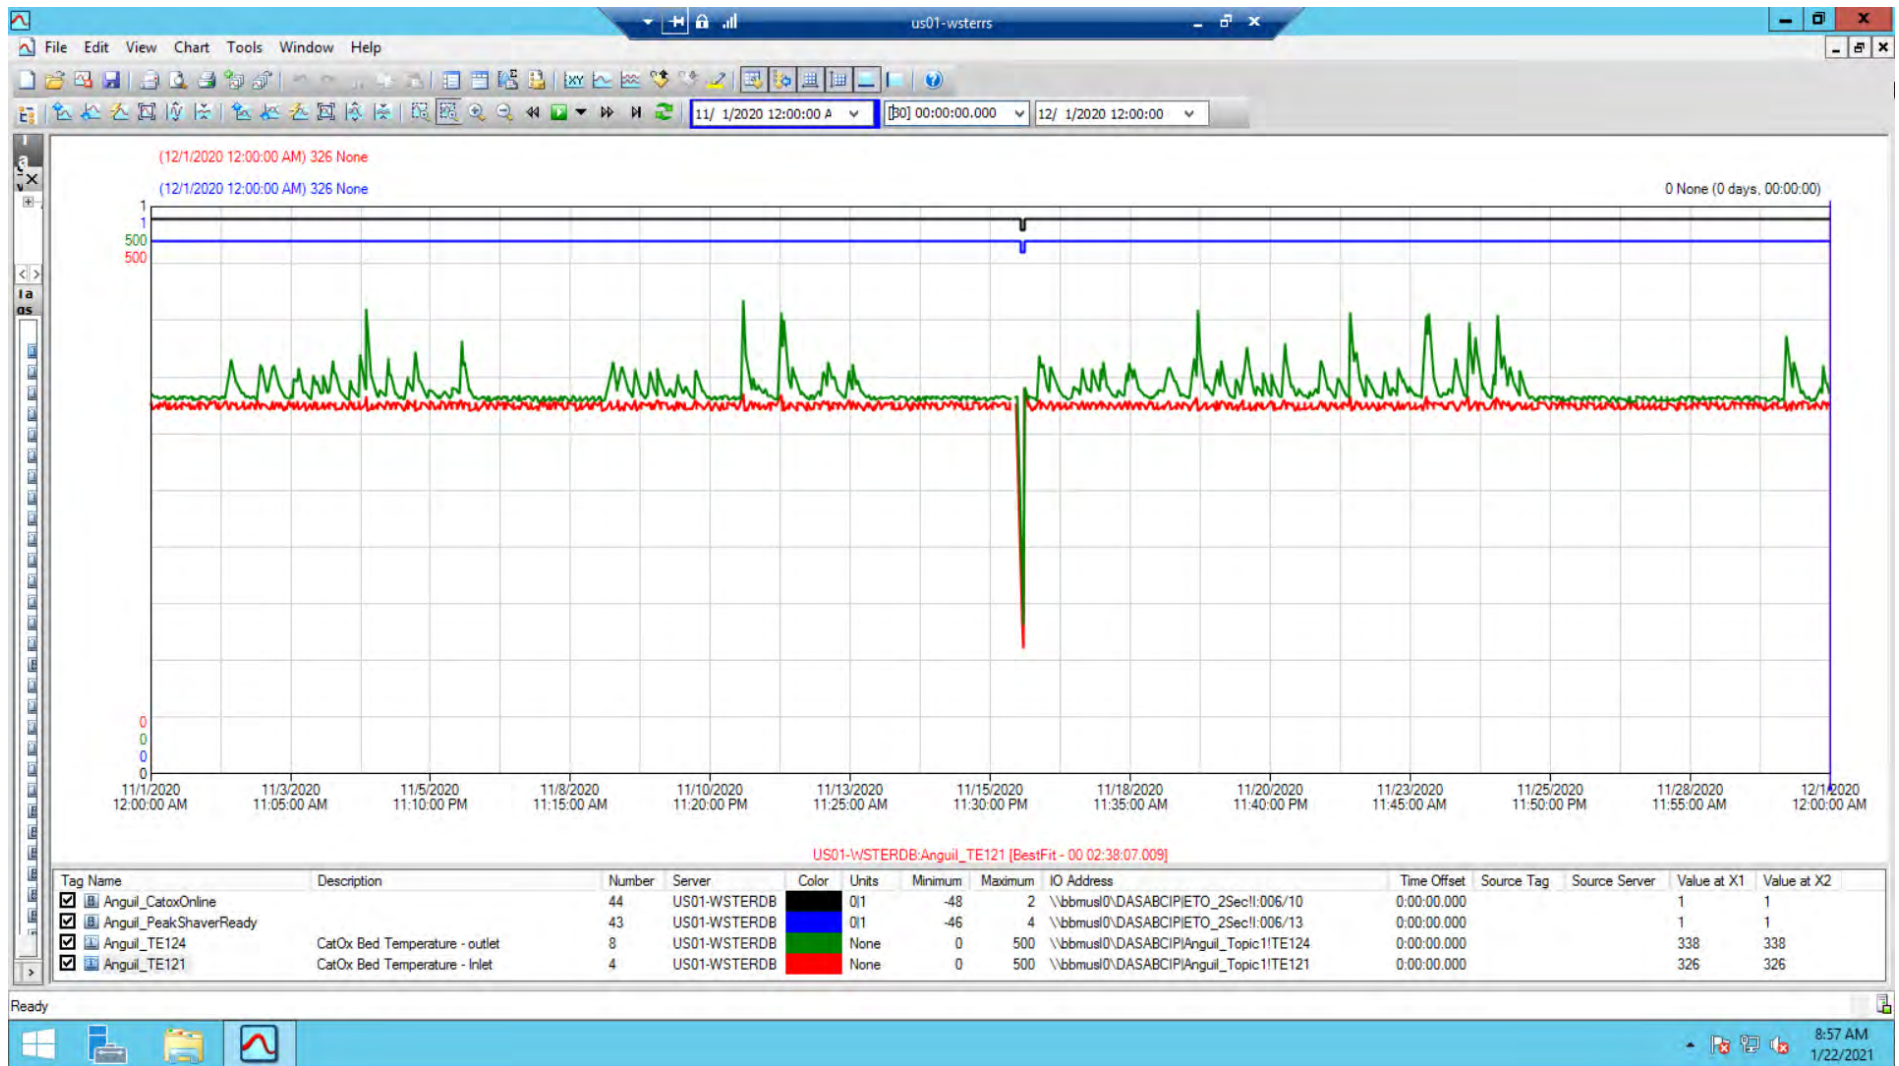



# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Nov 2020





# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020



# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020





# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020





# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020



# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020





# B Braun Medical Allentown Facility (Anguil CatOx Temperatures (degrees F)) – Dec 2020

